

PRECISION NOISE GENERATOR 8057A



HEWLETT  PACKARD

CERTIFICATION

The Hewlett-Packard Company certifies that this instrument was thoroughly tested and inspected and found to meet its published specifications when it was shipped from the factory. The Hewlett-Packard Company further certifies that its calibration measurements are traceable to the U.S. National Bureau of Standards for AC measurements and the Physikalisch Technische Bundesanstalt for DC measurements to the extent allowed by the Bureau's calibration facility.

WARRANTY AND ASSISTANCE

All Hewlett-Packard products are warranted against defects in materials and workmanship. This warranty applies for one year from the date of delivery, or, in the case of certain major components listed in the operating manual, for the specified period. We will repair or replace products which prove to be defective during the warranty period. No other warranty is expressed or implied. We are not liable for consequential damages.

For any assistance contact your nearest Hewlett-Packard Sales and Service Office. Addresses are provided at the back of this manual.

**MODEL 8057A
PRECISION NOISE GENERATOR**

SERIAL PREFIXED: G910

This manual is appropriate to instruments
with the serial number prefix:

1147G and below

CONTENTS

Section I	General Information	Page
1-1	Introduction	1-1
1-7	Options	1-1
1-9	Accessories Available	1-1
1-11	Manual Identification	1-1
1-13	Ordering Additional Manuals	1-1
Section II	Installation	
2-1	Initial Inspection	2-1
2-4	Preparation for Use	2-1
2-6	Power Cable	2-1
2-8	Environment	2-1
2-10	Operating Location	2-1
2-12	Repacking	2-2
Section III	Operating Instructions	
3-1	General	3-1
3-3	Internal Operation	3-1
3-5	External Filter	3-1
3-7	External Clock	3-1
3-9	Gating	3-1
Section IV	Theory of Operation	
4-1	Introduction	4-1
4-3	The Shift Register	4-1
4-7	The Digital-To-Analog Converter	4-3
4-17	Smoothing Filter	4-5
4-20	Output Attenuator	4-5
4-23	Trigger Output	4-6
4-25	Binary Output	4-6
4-27	Automatic Start	4-6
4-29	Clock Generator	4-6
4-31	Gate	4-6
4-33	Detailed Circuit Description	4-6
4-34	Shift Register	4-6
4-38	Digital-To-Analog Converter	4-6
4-41	Summing Amplifier, Smoothing Filter and RC Network	4-6
4-45	Attenuator	4-7
4-47	Trigger Output Generator	4-7
4-49	Binary Output Amplifier	4-7
4-51	Automatic Start Logic	4-7
4-54	Clock Generator	4-7
4-58	Gate	4-7
4-60	Power Supply	4-7

CONTENTS

Section V	Maintenance	Page
5-1	Introduction	5-1
5-3	Testing	5-1
5-5	Instrument Cover Removal	5-1
Section VI	Replaceable Parts	
6-1	Introduction	6-1
6-3	Ordering Information	6-1
Section VII	Diagrams	
7-1	Introduction	7-1
Appendix I	Options	
A1-1	Option 001	A-1
A1-3	Option A85	A-1
A1-5	Option X95	A-1
Appendix II	Backdating	
A2-1	Models prior to Serial Number G910-00240	A-2
A2-3	Models prior to Serial Number G910-00150	A-2
A2-5	Models prior to Serial Number G910-00140	A-2
A2-7	Models prior to Serial Number 0963G-00390	A-2

ILLUSTRATIONS

Figure		Page
2-1	Noise Generator and Supplied Items	2-2
3-1	Front and Rear Panels	3-0
4-1	8057A Block Diagram	4-1
4-2	15-bit Pseudo Random Sequence	4-2
4-3	2-Stage Shift Register and D/A Converter	4-3
4-4	Comparison between the Frequency Spectrum of a Train of Pulses and the Equivalent Stretched Pulse	4-4
4-5	Weighting Resistors Chosen to give $(\sin x)/x$ Waveform	4-4
4-6	Time Waveform Generated by a Single Recirculating '1'	4-4
4-7	Time Waveforms Generated by the Binary Sequence	4-5
4-8	Output Spectrum of the D/A Converter	4-5
5-1	Organization of Tests	5-5
5-2	Troubleshooting Flow Chart	5-6
7-1	General Symbols and References	7-1
7-2	Microcircuit Packages	7-2
7-3	Assembly Location	7-3
7-4	Assembly 2 Component Layout	7-4
7-5	Assembly 2 Circuit Diagram	7-5
7-6	Assembly 3 Component Layout and Waveforms	7-6
7-7	Assemblies 3 and 7 Circuit Diagram	7-7
7-8	Assembly 1 Component Layout	7-8
7-9	Assemblies 4, 5 and 6 Circuit Diagram	7-8
7-10	Assembly 1 Circuit Diagram	7-9
A1-1	Option 001 Circuit diagram and Replaceable parts	A-1

TABLES

Table		Page
1-1	Specifications	1-2
5-1	Test Equipment	5-1
5-2	Performance Check: Sequence Length	5-2
5-3	Performance Check: Clock Frequency	5-2
5-4	Performance Check: Gated Operation	5-3
5-5	Performance Check: White Noise Linearity	5-3
5-6	Performance Check: Pink Noise	5-4
6-1	Replaceable Parts	6-2

GENERAL INFORMATION

1-1 INTRODUCTION

1-2 The Hewlett-Packard Model 8057A is a low-frequency, broad-band noise generator designed primarily for use in control system evaluations and applications requiring the simulation of pseudo-random disturbances.

1-3 The HP 8057A generates two kinds of noise signals: a two-level (binary) output signal and a continuous analog waveform which closely approximates Gaussian amplitude distribution. The binary signal is formed by a repeated series of noise patterns (or sequences) of known duration as generated by a shift register.

1-4 To produce the analog signal, a portion of the binary signal is fed to a digital-to-analog converter which acts as a digital filter to produce a $\sin x$ waveform (where x is an independent variable in the time domain) for the Gaussian output, further smoothing is carried out by an analog filter network to yield approximately rectangular "white" or "pink" spectrums (Table 1-1) as required.

1-5 The noise output has a line spectrum, the harmonic spacing being established by the combination of clock period (ΔT) and sequence length (N). The product of ΔT and N gives the duration of pseudo-random noise pattern, and its reciprocal is the lowest frequency in the spectrum.

1-6 The level of the Gaussian output (available from a front panel connector) is variable by means of an attenuator, and the output impedance may be set to 50 or 600 Ohms (by a switch on the front panel). The binary output is delivered at a fixed level of +10V from a rear panel connector.

1-7 OPTIONS

1-8 The HP 8057A Options are described in Appendix 1.

1-9 ACCESSORIES AVAILABLE

1-10 Electronic test equipment, cables, connectors, and other accessory items are available from Hewlett-Packard. For more information on specific items consult the Hewlett-Packard Catalog or Sales/Service Office.

1-11 MANUAL IDENTIFICATION

1-12 This instrument carries a 9-character serial number on the rear panel, the first 4 characters of which are termed the serial number prefix. If the prefix does not agree with that quoted on the title page, reference should be made to the change sheets which are to be found in Appendix 2. To obtain further information for any instrument, contact the nearest Hewlett-Packard Sales/Service Office; always specify the model number and complete serial number.

1-13 ORDERING ADDITIONAL MANUALS

1-14 One manual is shipped with each noise generator. Additional manuals may be purchased from the local Hewlett-Packard field office (see list at rear of this manual for addresses). Specify the model number complete serial number prefix, and HP stock number provided on the title page.

Table 1-1. Specifications

NOISE OUTPUT

Period of Noise Pattern: Approx. 2 (for external clock 1,048,575 x clock period).

Harmonic Spacing (Δf): Approx. 0.5 Hz (for external clock, $\Delta f = \frac{\text{clock frequency}}{1,048,575}$)

WHITE NOISE

Power Spectrum: Rectangular, low pass. Nominal upper limit frequency (3 dB point) is 26 kHz (or 1/20th of external clock frequency).

Effective bandwidth: 27 kHz. Spectrum is flat within ± 0.3 dB up to 15 kHz and more than 25 dB down at 52 kHz.

Power Density: $362 \times 10^{-6} \text{ V}^2/\text{Hz} = \frac{(\text{rms amplitude})^2}{\text{effect. bandwidth}}$

Crest Factor: 3.5

Probability Density Function: Near Gaussian

PINK NOISE

Power Spectrum: 3 dB/octave decreasing from 3 Hz to 20 kHz. Deviation from ideal decrease: ± 0.5 dB up to 15 kHz + 0 dB, - 1.5 dB at 20 kHz.

Intersection of White and Pink Noise Power Density Spectrum: Approx. 2.6 kHz.

Amplitude: 3,126 V rms $\pm 2\%$ (i.e. 129.9 dB above 1 μV) (open circuit).

Amplitude Attenuator: 0.1, 1 and 10 dB steps from 20 to 129.9 dB above 1 μV . Overall attenuator accuracy ± 0.5 dB.

Output Impedance: 50 Ω or 600 $\Omega \pm 3\%$.

DC Offset: $< \pm 50$ mV from 32°F to 122°F (0°C to 50°C).

BINARY OUTPUT

Output Signal: Pseudo-random binary sequence (NRZ).
Clock rate: 520 kHz (or external clock). Sequence length (clock periods per sequence): 1,048,575.

Amplitude: 10V $\pm 10\%$. (open circuit).

Output Impedance: Approx. 600 Ω

Rise and Fall Times: < 70 nsec.

TRIGGER OUTPUT

Positive trigger pulse indicates period of the noise pattern.

Trigger Pulse Amplitude: Approx. 10 V.

Output Impedance: Approx. 1 k Ω .

Trigger Pulse Width: 2 μsec . (or equal to clock period of external clock frequency).

EXTERNAL CLOCK INPUT

(Used only for white noise output, refer to paragraph 4-57).

Pos. Clock Pulses (min. + 2 V; max. + 20 V amplitude)
(sine wave at least 4 V peak to peak)

Max. Clock Rate: 1 MHz

Min. Pulse Width: 30 ns.

Input Impedance: Approx. 1 k Ω .

GATE INPUT

Enable: + 4.5 to + 12 V.

Inhibit: - 1 to + 2.4 V (or connect to ground -2.5 mA is then delivered from the GATE INPUT connector).

Table 1-1 Specifications (cont'd)

OUTPUT TO EXTERNAL FILTER

(For noise spectra other than white or pink, connect external filter).

Pin 3	+ 15 V, output current 100 mA
Pin 1	- 15 V, output current 100 mA
Pin 2	Floating ground
Pin 4	Noise Output
Pin 5	Input from external filter.

GENERAL

Environment: Ambient temperatures from 0°C to 50°C and relative humidity to 95% at 40°C.

Power: 115 V or 230 V + 10%, - 15%, 50 Hz to 400 Hz, 14 VA.

Dimensions: Standard HP half module; 155 x 190 x 279 mm (6 x 7.75 x 11 inches).

Weight: Net, 3.5 kg (8 lbs); Shipping, 4.5 kg (10lbs).

2-1 INITIAL INSPECTION

2-2 Inspect the instrument for physical damage. After complying with the instructions given in paragraph 2-5, connect the instrument to the supply and carry out operational checks as soon as possible after delivery. If physical damage is evident, or if the instrument does not meet specifications when received, notify the carrier and the nearest Hewlett-Packard Sales/Service Office (see list at rear of this manual). The Sales/Service Office will arrange for repair or replacement without waiting for settlement of a claim with the carrier. The certification and warranty statements for all HP instruments are on the inside front cover of this manual.

2-3 The instrument is delivered complete with the following items (figure 2-1):

	Part Number
Manual	08057-90001
Power Cord	8120-1349
Fuse, 125mA, 230V operation	2110-0064
Fuse, 250mA, 115V operation	2110-0774
Board Extender, 15 pin	5060-0049
Board Extender, 18 pin	5060-1742

2-4 PREPARATION FOR USE

2-5 The Model 8057A may be operated from an ac source of 115 volts or 230 volts (+10%, -15%) at 50 Hz to 400 Hz. The power dissipation is 14VA. Carry out the following procedure if it is required to change the operating voltage:

- a. Disconnect the instrument from the supply.
- b. Remove the fuse and replace with a fuse of the appropriate value (paragraph 2-3).
- c. Insert a narrow-blade screwdriver into the rear-panel voltage selector switch and slide the switch to expose the required setting (i. e. 115 or 230).

- d. Insert the power cable and connect to the supply.

CAUTION

Be sure that the number visible on the voltage slide switch and the fuse value correspond to the line voltage used before operating the instrument; otherwise, the instrument may be damaged.

2-6 POWER CABLE

2-7 The Model 8057A is equipped with a 3-wire power cable which, when connected to an appropriate receptacle, grounds the instrument, its cabinet and panel. To preserve this protection feature when operating the instrument from an outlet without a ground connection, use an appropriate adapter and connect the ground lead to an external ground.

2-8 ENVIRONMENT

2-9 Conditions during storage and shipment should be limited as follows:

- a. Minimum temperature: -40°C (-40°F).
- b. Maximum temperature: 75°C (167°F).

2-10 OPERATING LOCATION

2-11 The 8057A can be used on the bench or rack-mounted. When used on the bench it can be inclined for convenient operation of the front panel controls by means of the folding stand. Instructions for rack mounting are included in the rack mounting kit.

2-12 REPACKING

2-13 The original shipping carton and packing material can be used for reshipment. The Hewlett-Packard Sales and Service Office will also provide infor-

mation and recommendations on material to be used if the original packing material is not available or is not reusable. If the instrument is to be shipped to a Hewlett-Packard Sales/Service Office for repair, attach a tag showing owner, model, serial number and repairs required.



Figure 2-1 Noise Generator and Supplied Items





FRONT PANEL

- 1 LINE ON — OFF control. Latching push button. When operated, the neon indicator lamp (above) glows.
- 2 NOISE SELECTION control. Push buttons, push — pull coupled for selection of either WHITE or PINK noise.
- 3 IMPEDANCE SELECTION control. Push buttons, push — pull coupled for selection of either 50 or 600Ω output impedance.
- 4 NOISE OUTPUT connector. Selected noise (WHITE OR PINK) is available at this BNC connector.
- 5 10dB ATTENUATOR switch. Attenuates output noise in 10dB steps.
- 6 1dB ATTENUATOR switch. Attenuates output noise in 1dB steps.
- 7 0.1dB ATTENUATOR switch. Attenuates output noise in 0.1dB steps.

REAR PANEL

- 8 CONNECTION to 8055A or any other external filter.
- 9 GATE INPUT connector. Any external signal level between -1V and +2.8V disables noise output.
- 10 CLOCK INPUT connector for external clock signal. NOTE: To be used only for WHITE noise output.
- 11 BINARY OUTPUT connector. Pseudo-random binary sequence of 1,048,575 bits. Amplitude: 10V.
- 12 CLOCK SELECTION switch. Slide switch selects internal or external clock.
- 13 TRIGGER OUTPUT connector. Positive going trigger pulse ($\approx 10V$), indicating the period of noise pattern.
- 14 OUTPUT CONNECTION switch. Slide switch connects noise output signal to the front-panel OUTPUT BNC either directly or via Model 8055A or any other external filter.
- 15 FUSE HOLDER
- 16 POWER SELECTION switch. Slide switch to select desired supply voltage.
- 17 POWER receptacle. The Model 8057A is powered by 230 or 115V AC, 50 to 400 Hz ac supply.



Figure 3-1 Front and Rear Panels

3-1 GENERAL

3-2 Refer to the control identification diagram (figure 3-1) and install the instrument as explained in Section II.

3-3 INTERNAL OPERATION

3-4 Set the controls as follows:

- a. Depress LINE ON/OFF button 1 and verify that the lamp lights.
- b. Press required NOISE button 2.
- c. Press required IMPEDANCE button 3.
- d. Set required output level on controls 5, 6 and 7.
- e. Set switch 12 to INT.
- f. Set switch 14 to NORMAL.

3-5 EXTERNAL FILTER


3-6 If the output is to be processed by an external filter, connect the filter to the 5-pin connector 8 on the rear panel (refer to table 1-1 for the pin allocation), and set switch 14 to EXT FILTER.

3-7 EXTERNAL CLOCK

3-8 Set up as in paragraph 3-3, set switch 12 to EXT and apply a suitable clock signal (table 1-1) to connector 10. The external clock may be any frequency up to 1 MHz, but refer to paragraph 4-18 (if it is intended to use frequencies below 520 kHz) and to paragraph 4-16. The external clock facility should **not** be used when pink noise is required (see paragraph 4-57).

3-9 GATING

3-10 The noise generator may be gated off by applying a TTL low state (or ground connection) to connector 4. The noise generator restarts when the TTL level goes high (or when the ground connection is removed).

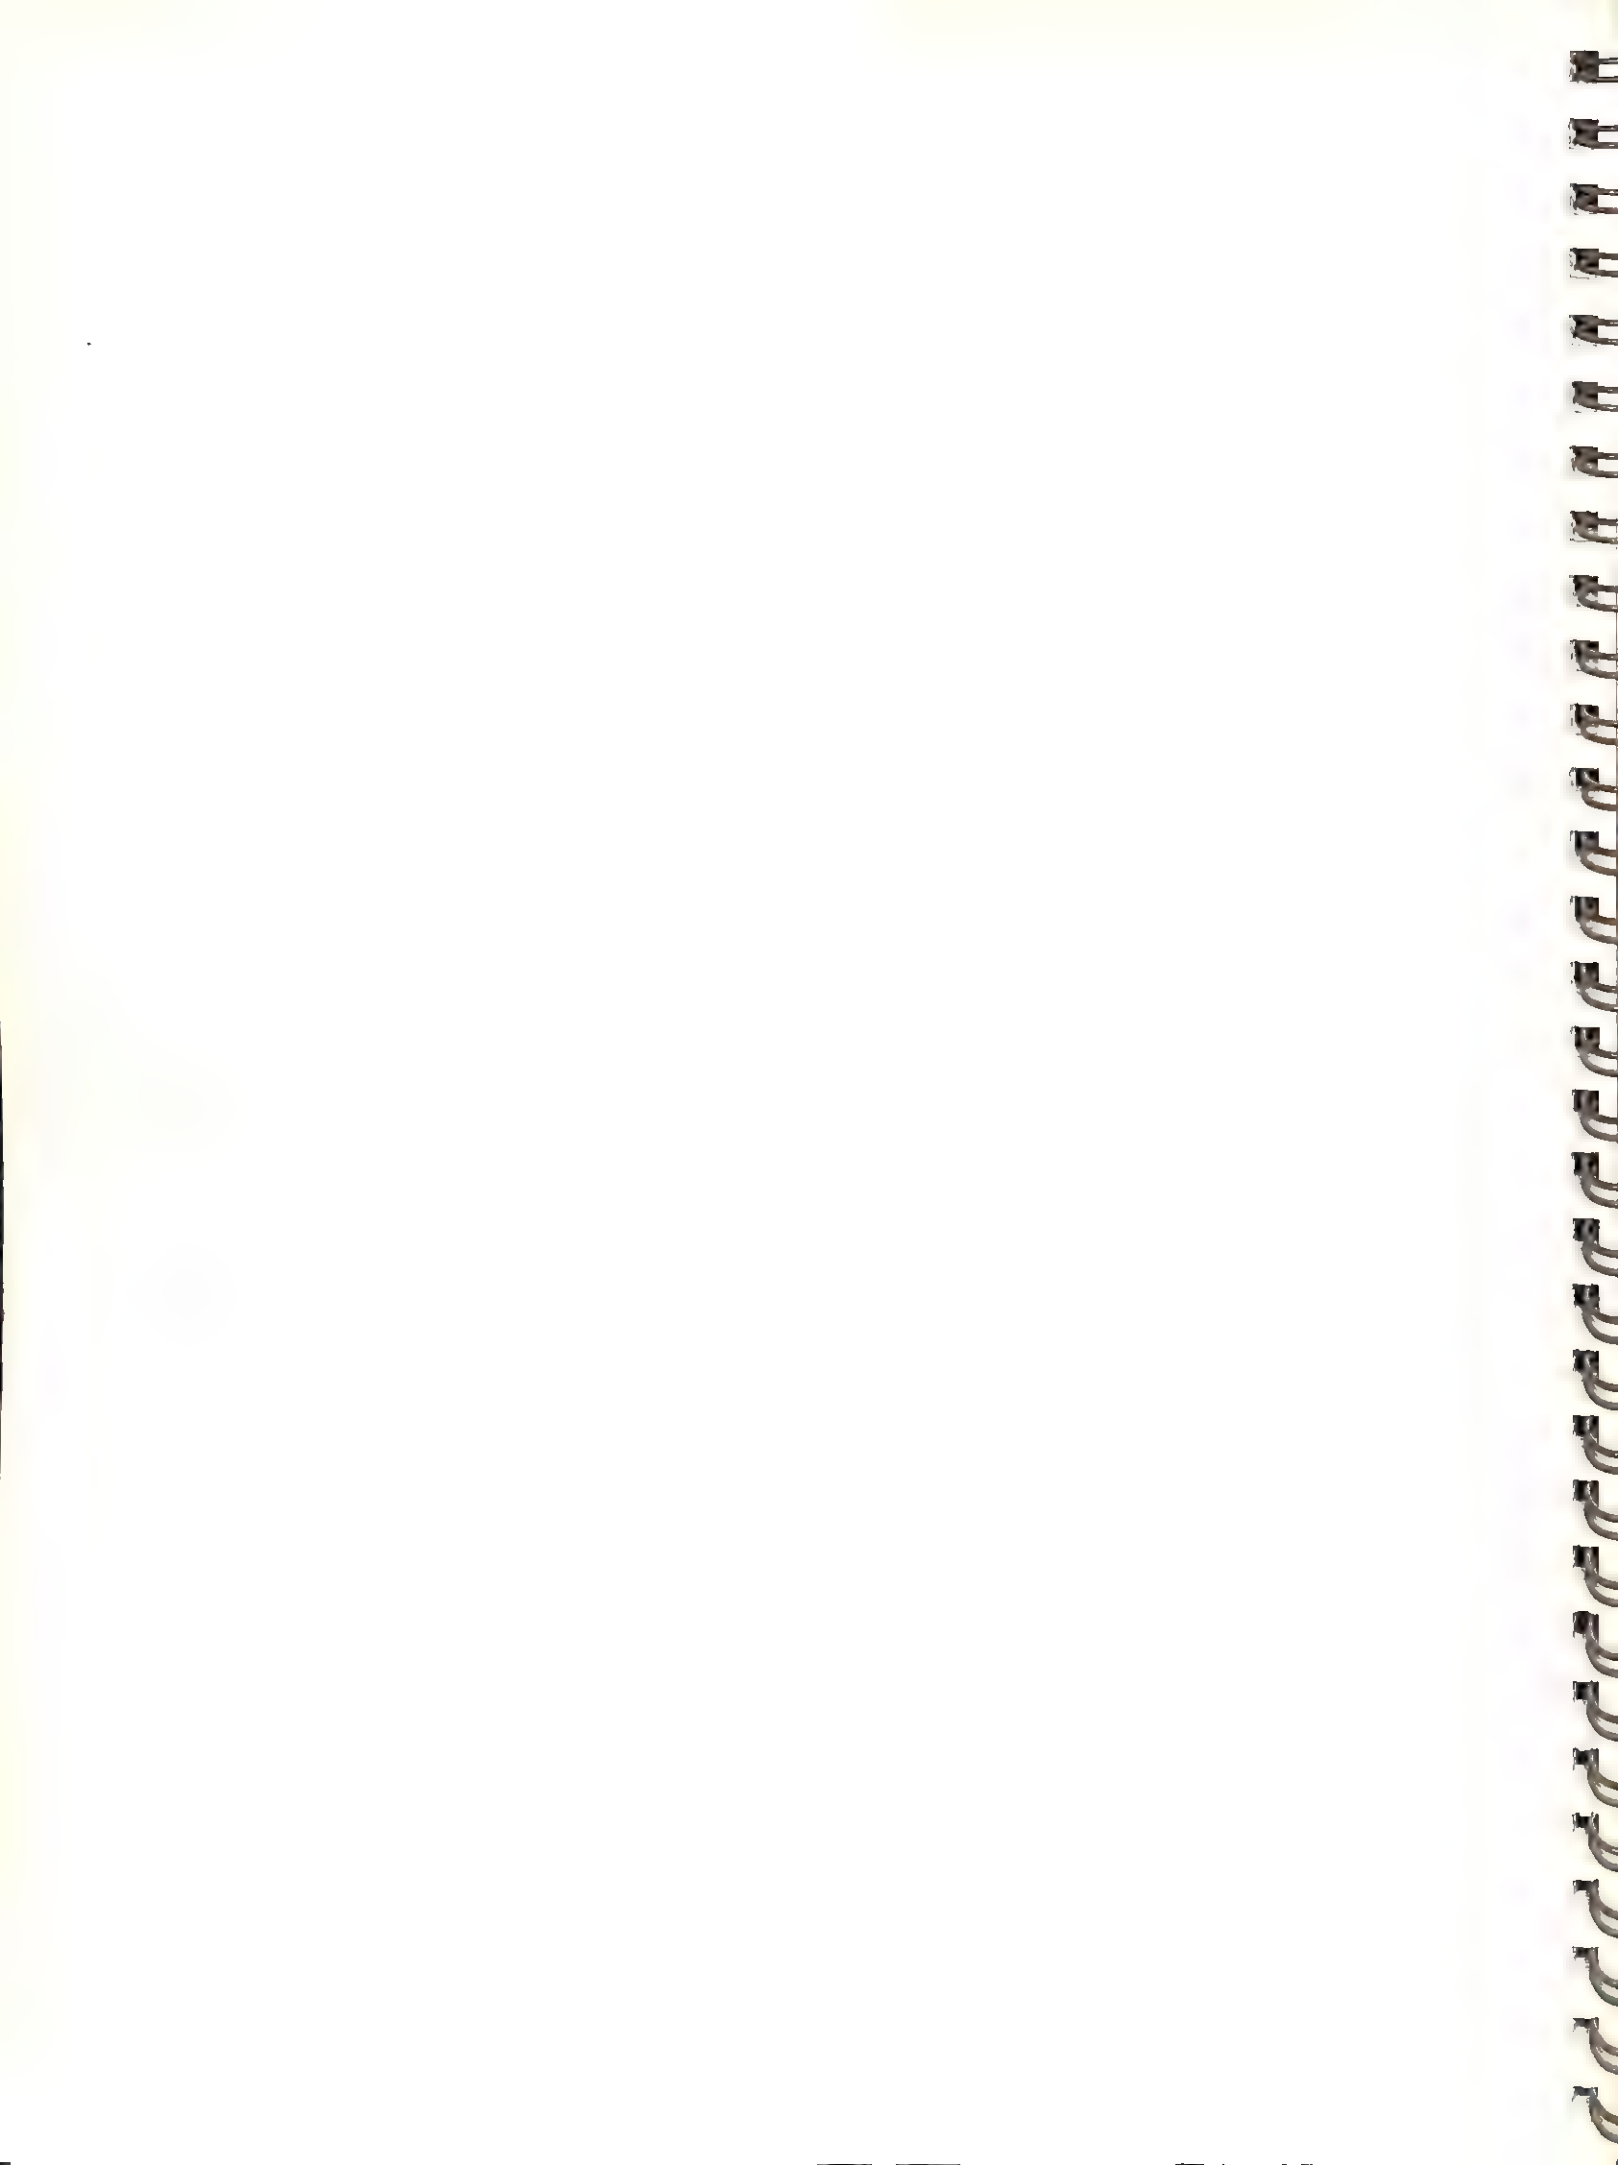

4-1 INTRODUCTION

4-2 This section contains a brief description of the way in which the 8057A works, the explanation is based on the block diagram in figure 4-1.

4-3 The Shift Register

4-4 The shift register is a series of flip-flops each of which acts as a store for binary digital information ('bit'). Each stage can be in one of two stable states, thus

it is said to contain a '1' bit if in the set state and a '0' bit if reset.

4-5 The shift register stages are connected in cascade so that on receipt of a clock pulse the binary combination is moved along one stage, i. e., each stage assumes the previous state of the stage driving it. If, as shown in figure 4-2, the output of two stages is fed back through an exclusive-or gate to the first stage, the register will generate a repeated series of identical sequences, known as a pseudo random binary sequence (p.r.b.s.).


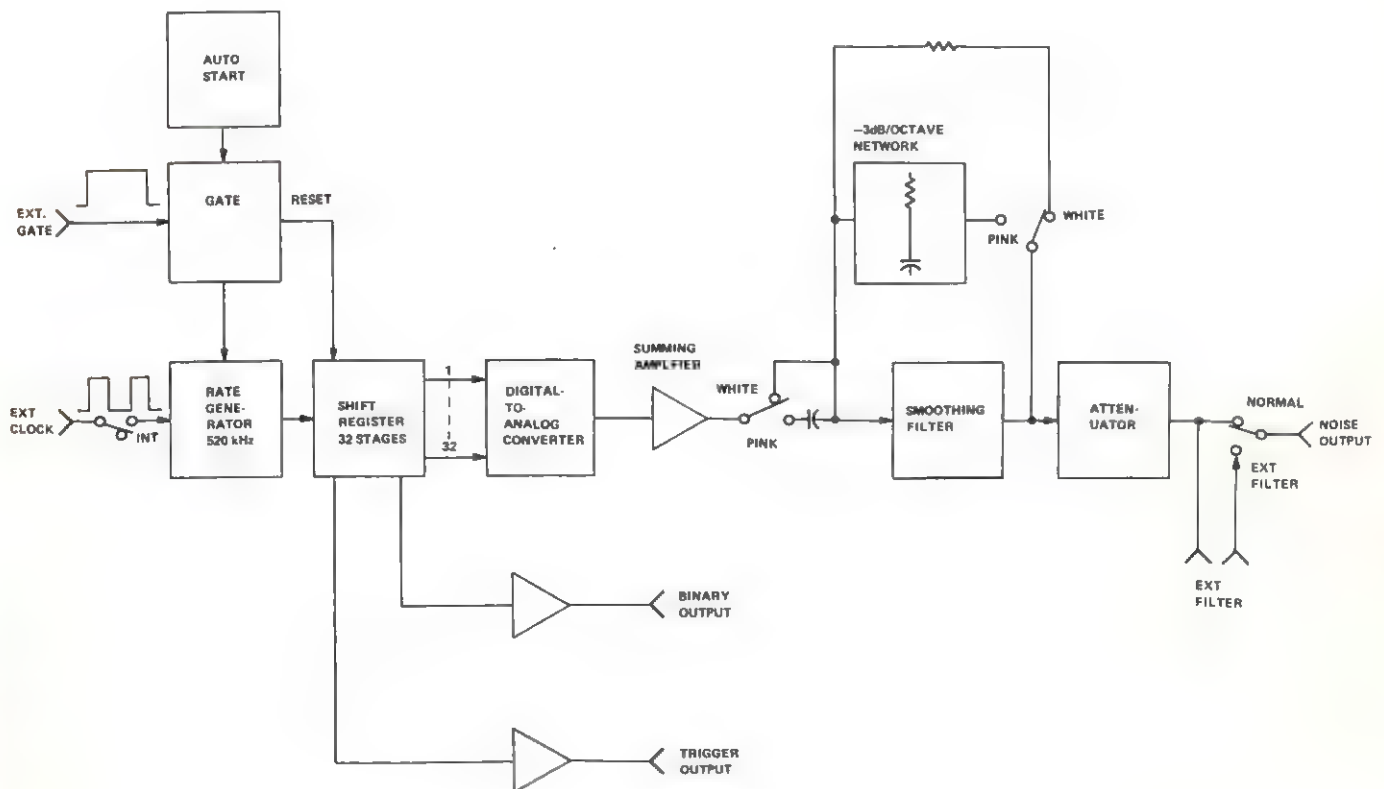


Figure 4-1 8057A Block Diagram

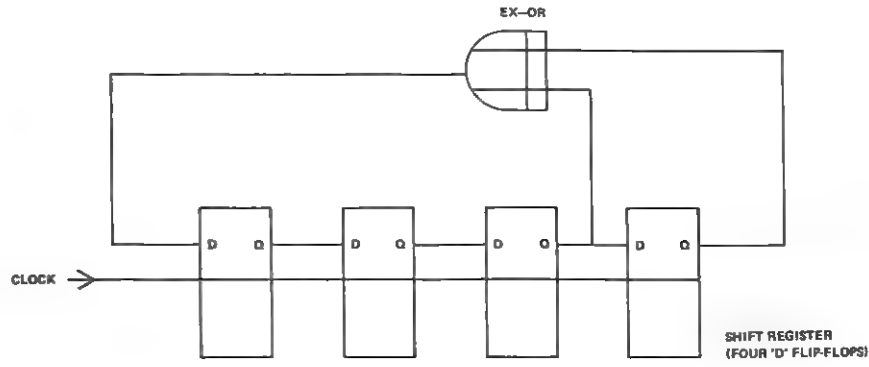

INITIAL STATE

1 0 0 0

SUBSEQUENT STATES
AFTER CONSECUTIVE
CLOCK PULSES:

1ST	0	1	0	0
2ND	0	0	1	0
3RD	1	0	0	1
4TH	1	1	0	0
5TH	0	1	1	0
6TH	1	0	1	1
7TH	0	1	0	1
8TH	1	0	1	0
9TH	1	1	0	1
10TH	1	1	1	0
11TH	1	1	1	1
12TH	0	1	1	1
13TH	0	0	1	1
14TH	0	0	0	1
15TH	1	0	0	0

PRBS

Figure 4-2. 15-bit Pseudo Random Sequence

It can be seen from figure 4-2 that the sequence will repeat itself every 15th clock pulse for a register of just 4 stages, also, it should be noted that the register never achieves a state with all stages at binary 0. For a shift register of n stages, the sequence length is $2^n - 1$.

4-6 In the HP Model 8057A Noise Generator the first 20 stages of a 32-stage register generate the p.r.b.s. (the output of the first 20 and remaining 12 stages is used to formulate the $(\sin x)/x$ waveform). Thus, under normal working conditions, the sequence will repeat itself after 1,048,575 clock pulses; for test purposes, however, the active length of the register is shortened to 10 stages, which gives a sequence of 1,023.

4-7 The Digital-to-Analog (D/A) Converter

4-8 The outputs of each of the 32 stages of the shift register are fed in parallel to the D/A converter about to be described in order to form a Gaussian signal.

4-9 However, consider first a simplified method of converting a binary signal into a multilevel analog waveform. Figure 4-3 shows a two-stage register coupled to weighting resistors of the same value. The circuit is so arranged that the current flowing through each resistor depends upon the state ('1' or '0') of its associated stage. Thus, the possible combinations with two stages are:

1. No current (both stages in '0' state).
2. One unit of current (either stage in '1' state).
3. Two units of current (both stages in the '1' state).

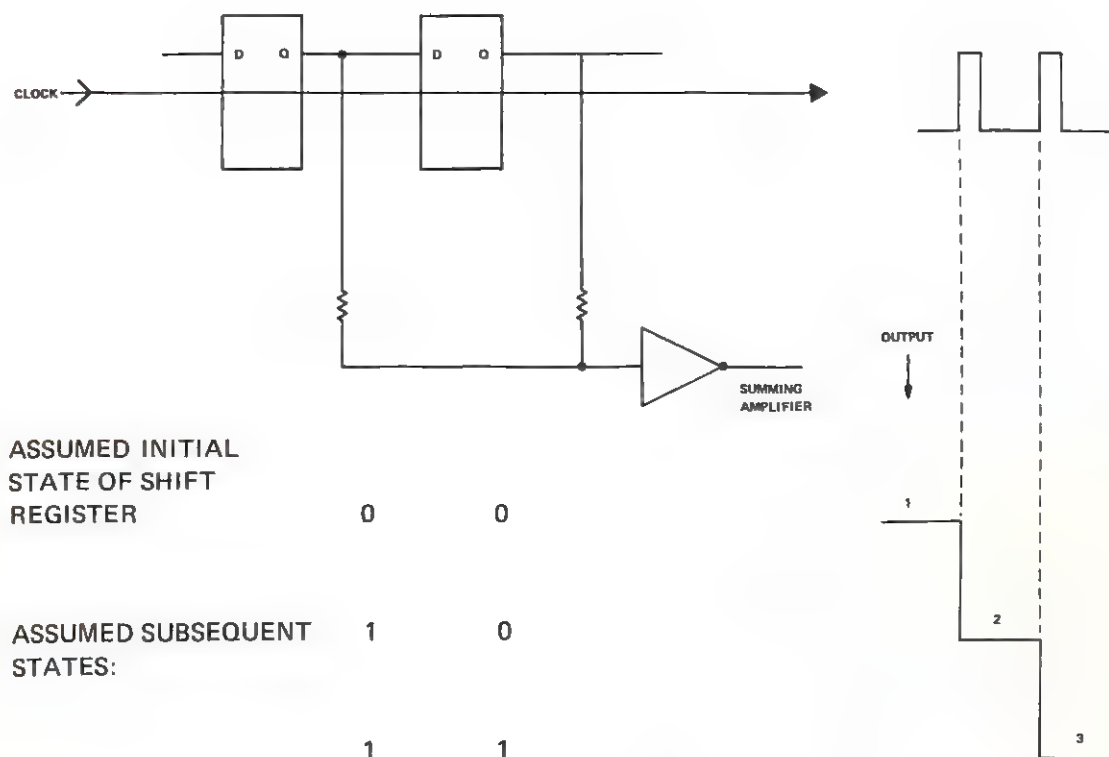


Figure 4-3 2-Stage Shift Register and D/A Converter

Hence the signal at the summing point can, at any given time, have one of three values, depending on the combination of bits in the two stages. Note that, as in normal shift register function, the pattern changes only when a clock pulse is received.

Clearly then, with a large number of shift register stages contributing to the output, the number of possible levels is increased. The device therefore derives a multi-level waveform from a two-level signal.

4-10 Now consider a single '1' pulse of width ΔT , applied to a 10-stage register (figure 4-4), driving ten identical loads. There is now no change in the output level at the summing point because the '1' passes from one state to the next. The output from the ten stages is therefore a stretched rectangular pulse. With clock pulses at intervals of ΔT , the width of the output pulse will be $10 \Delta T$.

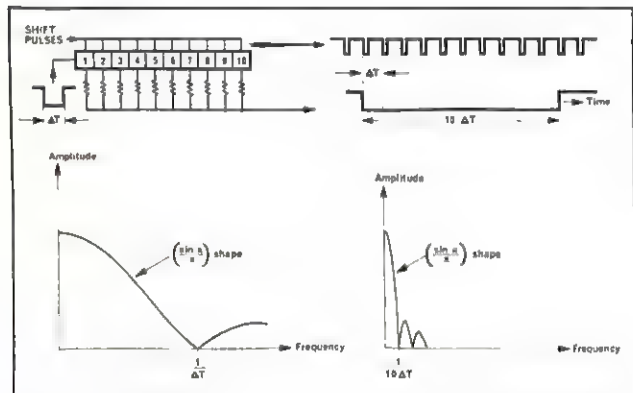


Figure 4-4. Comparison between the Frequency Spectrum of a Train of Pulses and the Equivalent Stretched Pulse.

4-11 A train of pulses of width ΔT has a $(\sin x)/x$ shaped spectrum with the first null occurring at the frequency $1/\Delta T$. Clearly, for a train of stretched pulses as in figure 4-4, the frequency of the first null is $1/10\Delta T$. That is to say that the signal band width has been reduced by a factor of 10.

4-12 In the 8057A the load resistors of the 32-stage shift register are chosen so that the current contribution at the summing point is graded, from one end of the shift register to the other, to follow the $(\sin x)/x$ curve (figure 4-5).

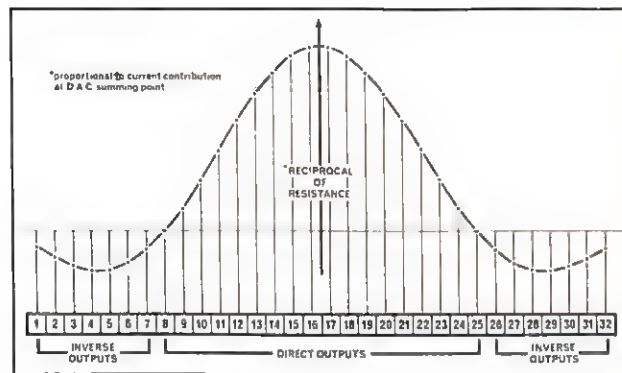


Figure 4-5. Weighting Resistors Chosen to give $(\sin x)/x$ Waveform

4-13 As shown in figure 4-5, the $(\sin x)/x$ curve is incomplete and stops short at a point in the second lobe on either side of the center line; this is because of the practical limitations on the size of the shift register. Note that the contributions to the signal made by the first and last seven groups of resistors is required to be the opposite polarity to that made by the resistors in the central group. This is achieved by supplying these two groups of resistors with the complement output signals from the respective register stages.

4-14 Therefore a single '1', starting at one end of the register and being conveyed (by a series of clock pulses), will generate a waveform as shown in figure 4-6 (as is the case when the 8057A is set to TEST).

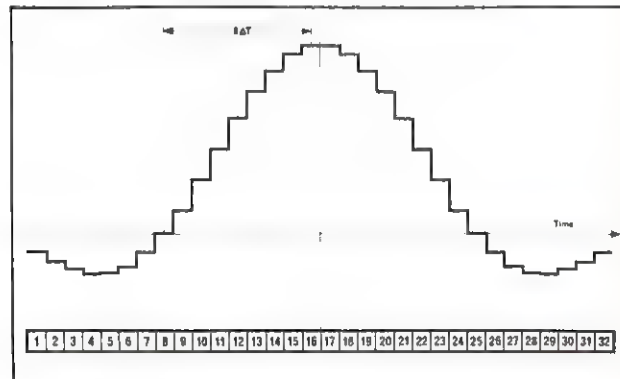


Figure 4-6. Time Waveform Generated by a Single Recirculating '1'.

4-15 In the normal mode the 20 active stages of the 8057A shift register generates the p.r.b.s. which is shifted throughout the complete length of the 32-stage register. The number of ones contributed to the output at any given time depends on the p.r.b.s. (and, therefore, also on the feedback loop which introduces a binary '1' at the input of the first register stage). Thus, a series of $(\sin x)/x$ curves will be apparent at the output of the D/A converter (figure 4-7) the sum of which results in a noise signal with an almost rectangular frequency characteristic, as shown in figure 4-8.


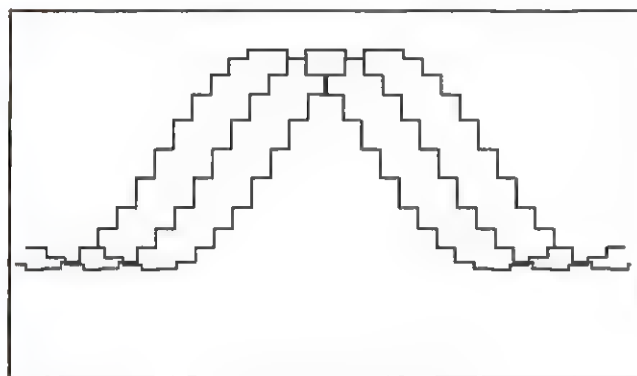


Figure 4-7. Time Waveforms generated by the Binary Sequence

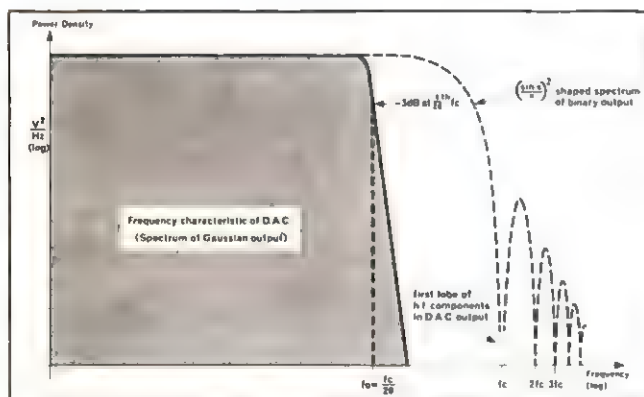

DAC = Digital-to-Analog Converter

Figure 4-8 Output Spectrum of the D/A Converter

Owing to the limited size of the shift register, which results in truncation of the $(\sin x)/x$ curve, the corner of the frequency characteristic is not perfectly square. The high frequency components in the output spectrum are caused by abrupt changes in the output levels as the pulses pass along the register and are removed by a smoothing filter (paragraph 4-17).

4-16 The design of the filter (shift register and D/A converter) is such that the half-power frequency of the Gaussian noise spectrum occurs at 1/20th of clock frequency. For example, with the internal clock frequency of 520 kHz, the relative power at 26 kHz is -3dB. The output from the digital filter is a multi-level signal having an approximately Gaussian distribution of amplitude and it is distinguished from a conventionally low-pass filtered signal only by the abrupt steps between levels. The amplitude of the probable density function (P.D.F.) of the multi-level signal is not significantly affected by the values of the weighting resistors assigned to the various shift register stages. The Gaussian nature of the P.D.F. arises mainly from the apparent randomness of the changing pattern of the binary signal within the shift register. Thus the P.D.F. attains a closer approximation to the Gaussian curve as the sequence length, and hence the randomness is increased. Note that the clock frequency (f_c) affects the spacing (Δf) between the harmonic components, and also the value of the half-power frequency (f_0).

4-17 Smoothing Filter

4-18 As previously mentioned, unwanted high frequency components in the output from the digital filter summing amplifier are removed by an analog smoothing filter. In analog computing applications, time derivatives of signals occur frequently and, whenever a signal has sharp edges, there is a danger that the derivatives could cause overload. In the case of a stepped waveform, with its very fast transit times, even the first derivatives would be a series of very large amplitude spikes. For this reason, a second order analog filter is included in the 8057A to remove the sharp edges from the digital filter output waveform. As a result, neither the first nor the second time derivatives of the waveform yield sharp spikes. The P.D.F. for both derivatives is, therefore, reasonably Gaussian. Note that, when operating from an external clock with a frequency lower than the 520 kHz of the internal clock, the output becomes more and more step-like.

4-19 A circuit providing a 3dB per octave attenuation may be switched into the smoothing filter if a narrower ('pink') spectrum is required instead of the broader ('white') spectrum.

4-20 Output Attenuator

4-21 The output signal from the smoothing filter is applied to the attenuator which provides an output from 20 to 129.9dB above $1\mu V$ in 0.1dB steps.

4-22 For spectra other than those for white or pink, an external filter can be connected between the smoothing amplifier and the attenuator.

4-23 Trigger Output

4-24 A circuit is incorporated which outputs a trigger pulse when the first 20 stages of the shift register assume a particular content. The trigger thus identifies a particular event in the p.r.b.s. which may then be regarded as the 'start' and 'end' of the sequence.

4-25 Binary Output

4-26 The binary amplifier receives the p.r.b.s. from the output of the last stage of the shift register. The pulse sequence is amplified to a fixed output of 10 volts with an open circuit impedance of approximately 600 Ohms.

4-27 Automatic Start

4-28 Under normal working conditions, the 8057A shift register could not set itself to an all zero state. There is, however, a possibility that directly after switching the instrument on, all active stages of the shift register could assume the '0' state. This situation is prevented by a reset pulse, generated by an automatic start circuit, which ensures that the register is always started with the same pattern of ones and zeroes.

4-29 Clock Generator

4-30 An oscillator and a pulse shaping network are used to generate the shift register clock pulses which have a frequency repetition rate of 520 kHz on internal operation. When triggering externally, the clock pulse rate is the same as that for the trigger up to a maximum frequency of 1 MHz.

4-31 Gate

4-32 Positive signals (or open circuit) applied to the rear panel 'Gate Input' connector will gate the instrument on to produce bursts of noise. After gating, the clock generator is stopped and the binary state of the register stages is reset to a fixed combination.

4-33 DETAILED CIRCUIT DESCRIPTION

4-34 Shift Register (Figure 7-5)

4-35 The shift register uses 16 integrated dual D-Type Flip-Flops (MC1 to MV16) (Figure 7-2) of which

MC1 to MC10 form the 20 active stages used to generate the p.r.b.s. Selected outputs are fed back to the first stage via the logic gate MC17, MC18 and MC19 and mode switch S1.

4-36 With the switch A2S1 (figure 7-3) set to N (for 'normal' operation), the active length of the register is 20 stages; when A2S1 is set to T (test), the active length is shortened to 10 stages. (See paragraph 4-6 for sequence length).

4-37 When the instrument is turned on, a pulse from Q37 of the automatic start circuit is applied to the set or reset of each flip-flop stage, so that the initial state of the shift register is set up as follows: 1111 1110 0011 1100 0000 0111 0001. The shift register also starts with this combination each time the clock generator is enabled by a gate signal. Clock pulses applied to each stage are from the output of Q45 and Q46.

4-38 Digital-to-Analog Converter (Figure 7-5)

4-39 Each D/A converter consists of a clamping network which uses a transistor (Q1 to Q30) and its associated resistances. The operating voltage (+11.7 volts) is supplied by the voltage source comprising of A3Q23 and Q25 (figure 8-10).

4-40 With the exception of stage 8 and 25, every stage is allocated a precision weighting resistor, R31 to R84. Stages 8 and 25 do not contribute to the signal because the output at that point corresponds to the zero crossing point of the $(\sin x)/x$ waveform (figure 4-6). The output from the weighting resistors is applied to the summing amplifier.

4-41 Summing Amplifier, Smoothing Filter and RC Network

4-42 The transistors Q1 and Q8 form the summing amplifier. The signal from the weighting resistors (R31 to R84) has a dc offset which is neutralized by the application of a negative voltage via R2 and R3. The white noise signal is adjusted for dc offset zero by R2 and the pink noise signal by R70. The white noise rms amplitude is adjusted by means of R68 and the pink noise rms amplitude is adjusted by R65. For white noise the filter is dc coupled to the summing amplifier, in PINK mode the filter is ac coupled to the summing amplifier via C12 and C13 and incorporates the RC network R43 to R52 and C15 to C23.

4-43 The input stage (Q1) is part of a differential amplifier, the output of which is further amplified by a

second differential amplifier (Q3 and Q4); the high frequency response is compensated by C1 and Q6. A balancing resistor R5 is connected between the collectors of Q1A-B to minimize the loading effects of Q3 and Q4 upon the amplitude. The emitter followers Q7 and Q8 are forward-biased by CR1 and CR2; the output signal (inverted with respect to the input signal) is connected via a feedback link, R12/R65, to the amplitude input.

4-44 The smoothing filter circuit is similar to that of the summing amplifier but is connected (by means of R19, R20, C4 and C5) as an active filter with a cut-off frequency of 110 kHz. In the PINK MODE the filter is ac coupled to the summing amplifier via C12 and C13 and incorporates the RC network R43 to R52 and C15 to C23.

4-45 Attenuator (Figure 7-9)

4-46 The attenuator is a ladder attenuator with separate controls for 10's, units and decimals of dB.

4-47 Trigger Output Generator (Figure 7-7)

4-48 The trigger is generated when the diodes CR1 to CR20 sense a high (or low) state at the Q (or the Q) outputs of the first 20 flip-flops. Therefore, at a particular shift register content (paragraph 4-37), the bias of Q19 becomes positive via R90, CR21 and CR22 (figure 8-8, sheet 3 of 4), thus opening this transistor and closing Q20. After the clock pulse has shifted the initial word, the positive bias at the base of Q19 is terminated, turning Q19 off and Q20 on, thus ending the trigger pulse.

4-49 Binary Output Amplifier (Figure 7-7)

4-50 With the binary output from stage 31 of the shift register in a low state, Q21 will conduct, keeping Q22 turned off. When the situation changes to high output, the voltage at R60 is clamped by the emitter base diode of Q22, and Q22 conducts.

4-51 Automatic Start Logic (Figure 7-5)

4-52 The automatic start circuit Q34/Q35 prevents the instrument from being disabled at switch-on by the shift register holding 32 zeroes.

4-53 The capacitor C2 is charged by Q34 via R94. When the voltage across C2 has reached the threshold of the uni-junction transistor Q35, it discharges through the network Q35, R95, CR23 and R98 and thus reduces

the emitter current of Q36. Q37 is turned on, sending a short reset pulse to the shift register.

4-54 Clock Generator (Figure 7-5)

4-55 The clock pulse is generated by the relaxation oscillator Q39 and Q41. Suppose that Q39 and Q41 are both off. C3 is then charged by Q40 at a constant rate, causing the junction of C3 and CR27 to fall towards the negative supply voltage. Consequently, the base emitter voltage of Q39 increases above the threshold and Q39 begins to conduct. As it does so, the base potential of Q41 falls and positive feedback is applied to the base of Q39; this results in both transistors being turned on rapidly.

4-56 A low impedance path now exists between the negative (top) end of C3 and the positive supply. C3 discharges rapidly causing the base emitter voltage of Q39 to fall below threshold. The trigger is a regenerative process in which both transistors are turned off rapidly. Pulse shaping is accomplished by the Schmitt trigger Q44 to Q46.

4-57 To operate from an external trigger, the clock generator is stopped by a negative potential applied from the voltage divider R112, CR30 and R113 via the rear panel INT/EXT switch to the base of Q39. Thus the voltage at C3 is clamped by the diodes CR28 and CR29 holding Q39 off. When a positive trigger signal is applied to J4, the Schmitt Trigger, (Q42/Q43), sends a short positive pulse (shaped by L1 and R117) via CR31 to the base of Q39 initiating one generator cycle. R107 is switched in parallel with R106 so that the charging current for C3 is increased thus permitting triggering frequencies up to 1 MHz. Note that, the pink output has the same RMS level as the white output and that consequently, the peak pink level is higher. Operation at clock frequencies other than the internal rate of 520 kHz can, therefore, lead to saturation of the amplifier. The external trigger, then, should not be used when pink noise is required.

4-58 Gate (Figure 7-5)

4-59 With the "Gate Input" grounded or in a low state (-1V to +2.8V) Q36, Q37 and Q38 are turned on, Q38 draws the current from Q40, hence the clock generator is stopped, and Q37 holds all 32 shift register flip-flops in a particular state (paragraph 4-44). Thus, when the gate voltage goes high, the shift register recommences from a particular state. The appropriate waveforms are shown in Figure 4-10.

4-60 Power Supply

4-61 The power supply assembly A1 provides the necessary operating voltages for the noise generator circuits. Since both the 15 volts positive and the 15volt negative circuits are similar, only the positive circuit will be described.

4-62 Rectifiers CR1 to CR4 supply the unregulated voltage to the regulator circuit. Transistors Q5 and Q6 make up to the differential amplifier which compares the line voltage level (adjustable by R10) to the reference voltage at CR6. Any variation of the +15 volt output is sensed by Q5 and Q6 to produce an error signal which is amplified by Q3 and Q1.

4-63 The current limiter Q4 is turned off under normal working conditions. Should the load current exceed 460mA, Q4 will be turned on by the voltage drop across R4. When Q4 turns on, Q1 and Q2 are turned off.

4-64 The shift register requires a potential difference of 5V, but, to allow proper operation of the summing amplifier circuit, the potential must be biased so that its return is at +10 volts. This is achieved by connecting the positive end of the potential difference established by Q12 to Q14 to the +15V line.

5-1 INTRODUCTION

5-2 The following information is presented in this section:

- a. Testing and Troubleshooting
- b. Removal and replacement of covers
- c. Recommended Test Equipment

5-3 TESTING

5-4 The performance checks described in the following tables are independent procedures which are intended to verify that the instrument is operating in accordance with the specification stated in table 1-1. These test procedures can also be used as a guide for troubleshooting in conjunction with figures 5-1 and 5-2. A list of recommended equipment required to test the 8057A appears in table 5-1.


5-5 INSTRUMENT COVER REMOVAL

5-6 The top, bottom and side covers can be separately removed to gain access to all assemblies. Each cover is secured by screws which are threaded into fasteners attached to the instrument castings.

Table 5-1 Test Equipment

Instrument	Minimal Requirements	Model Recommended
Pulse Generator	Pulse rate: 1 MHz Pulse width: 30 nS Amplitude: 0 to + 5 V	HP 8003A
Counter	Max.frequency: 1 MHz Ext. time: 1 MHz Base facility: 1 MHz Sensitivity: 1 V	HP 5254L
Oscilloscope	Max.trig.freq.: 20 MHz Sweep time: 20 nS Freq.range: dc to 20 MHz Sensitivity: 0.1 V/cm	HP 140A with plug-ins HP 1423A and HP 1402A
Wave Analyzer	Bandwidth: \pm 25 Hz Rejection: 50 dB	HP 302A

Table 5-2. Performance Check: Sequence Length

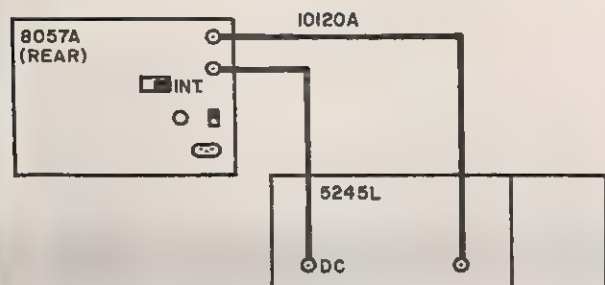

Set controls as follows:

8057A CLOCK SELECTOR SWITCH INT.

5245L PERIOD AVERAGE RANGE $\times 1$
 TIME BASE EXT.
 SENSITIVITY 1 volt rms.

5345L display should read:

$$262,144 = \frac{\text{sequence length} + 1}{4}$$

INTERNAL OPERATION

Set controls as follows:

8057A CLOCK SELECTOR SWITCH INT
 5245L FUNCTION Period av.
 TIME BASE range $\times 1$
 SENSITIVITY 1 mS
 1 volt rms.

5245L should indicate: 2016 mS \pm 20 mS

EXTERNAL OPERATION

Set controls as follows:

8057A CLOCK SELECTOR SWITCH EXT.
 8003A REP RATE SELECTOR 10 MHz
 REP RATE VERNIER CCW
 (Do not exceed 1 MHz)
 PULSE WIDTH SELECTOR 30 nS
 PULSE WIDTH VERNIER CCW
 AMPLITUDE 5 V
 1420A TRIGGER INT +
 MAGNIFIER $\times 1$
 SWEEP TIME 0.5 μ S

1402A FUNCTION A
 POLARITY +
 CH. A INPUT ON
 CH. A COUPLING DC
 CH. A SENSITIVITY 0.5 V/cm

5245L FUNCTION Period av.
 TIME BASE range $\times 1$
 SENSITIVITY 1 mS
 1 volt rms.

The 5245L reading should correspond to the following:

Trigger pulse period: $T = \frac{1,048,575}{\text{trigger freq.}}$

Table 5-3. Performance Check: Clock Frequency


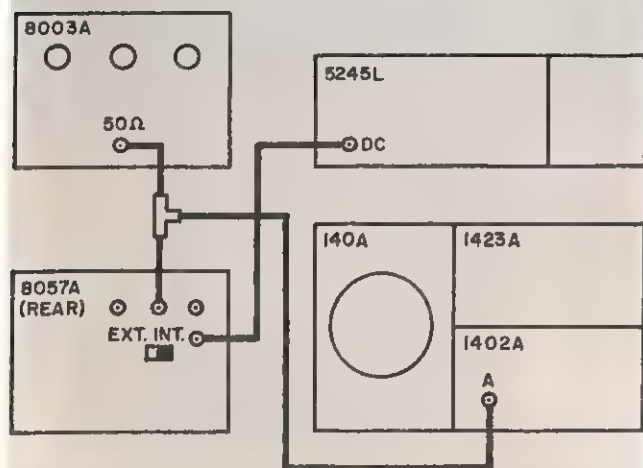


Table 5-4. Performance Check: Gated Operation

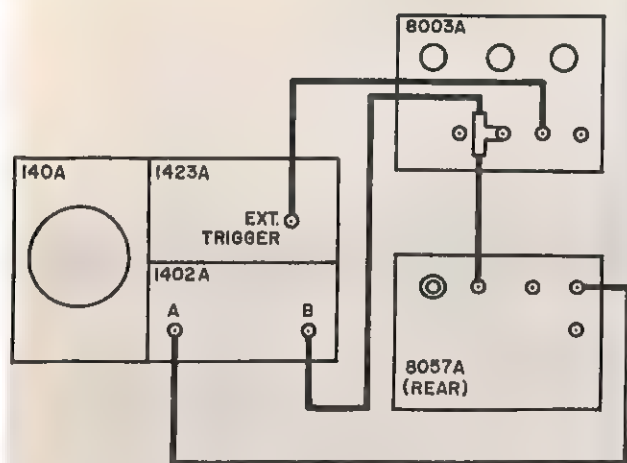


Set controls as follows:

8057A	CLOCK SELECTOR SWITCH	INT.
8003A	REP RATE SELECTOR	0.3 MHz
	REP RATE VERNIER	CCW
	PULSE WIDTH SELECTOR	0.1 mS
	PULSE WIDTH VERNIER	CCW
	AMPLITUDE	+ 2.3 volts
1420A	TRIGGER	EXT
	SWEEP TIME	20 μ S
1402A	FUNCTION	ALT
	POLARITY	+
	CH. A	5 V/cm
	CH. A COUPLING	DC
	CH. B	1 V/cm
	CH. B COUPLING	DC

Binary output signal should be enabled when the gate amplitude is $> +4.5$ volts and disabled when $< +2.8$ volts.

Table 5-5. Performance Check: White Noise Linearity

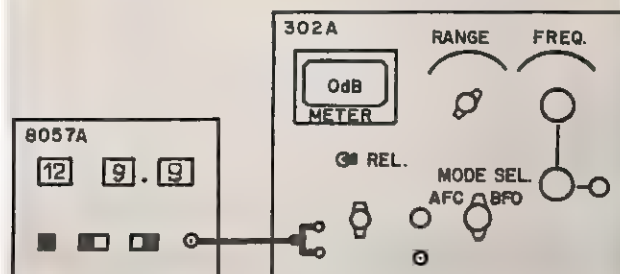

Set controls as follows:

8057A	ATTENUATOR	129.9 dB
	NOISE	WHITE
	IMPEDANCE	600 Ω
	S1 (mounted on assy A2)	T
302A	SCALE VALUE	RELATIVE
	MAX INPUT VOLTAGE	1 volt
	MODE SELECTOR	NORMAL
	FREQUENCY	0 Hz
	RANGE	300 mV

Increase the Wave Analyzer frequency until the meter indicates the first harmonic peak. Frequency reading should be about 500 Hz.


Set MODE SELECTOR SWITCH to AFC. Observe that the meter needle remains on top of the peak and then turn the setting to 0dB by means of the MAX. INPUT VOLT. AGE VERNIER.

Set MODE SELECTOR to NORMAL. Find the second harmonic by increasing the Wave Analyzer frequency until the next peak causes a deflection on the meter.

Set MODE SELECTOR to AFC. Meter should now indicate 0dB (± 0.3 dB). The harmonic spacing should be about 500 Hz.

Continue checking linearity and harmonic spacing up to 27 kHz.

Table 5-6. Performance Check: Pink Noise

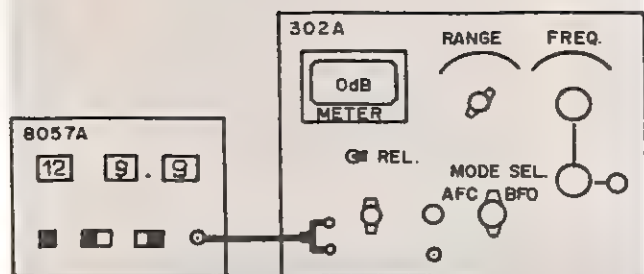

Set the controls as follows:

8057A	Noise	PINK
302A	MAX. INPUT VOLTAGE	3 volts
	SCALE VALUE	RELATIVE
	MODE SELECTOR	NORMAL
	FREQUENCY	0 Hz
	RANGE	300 mV

Increase the Wave Analyzer frequency until the meter indicates the first harmonic peak. Frequency reading should be about 500 Hz.

Set MODE SELECTOR SWITCH to AFC. Observe that the meter needle remains on top of the peak. Find the second harmonic (first octave). The meter should indicate -3dB ($\pm 0.5\text{dB}$).

Find fourth harmonic (second octave). Meter should indicate -6dB ($\pm 0.5\text{dB}$).

Result:

Harmonic spacing should be about 500 Hz. The spectrum should increase by 3dB per octave ($\pm 0.5\text{dB}$) up to 15 kHz.

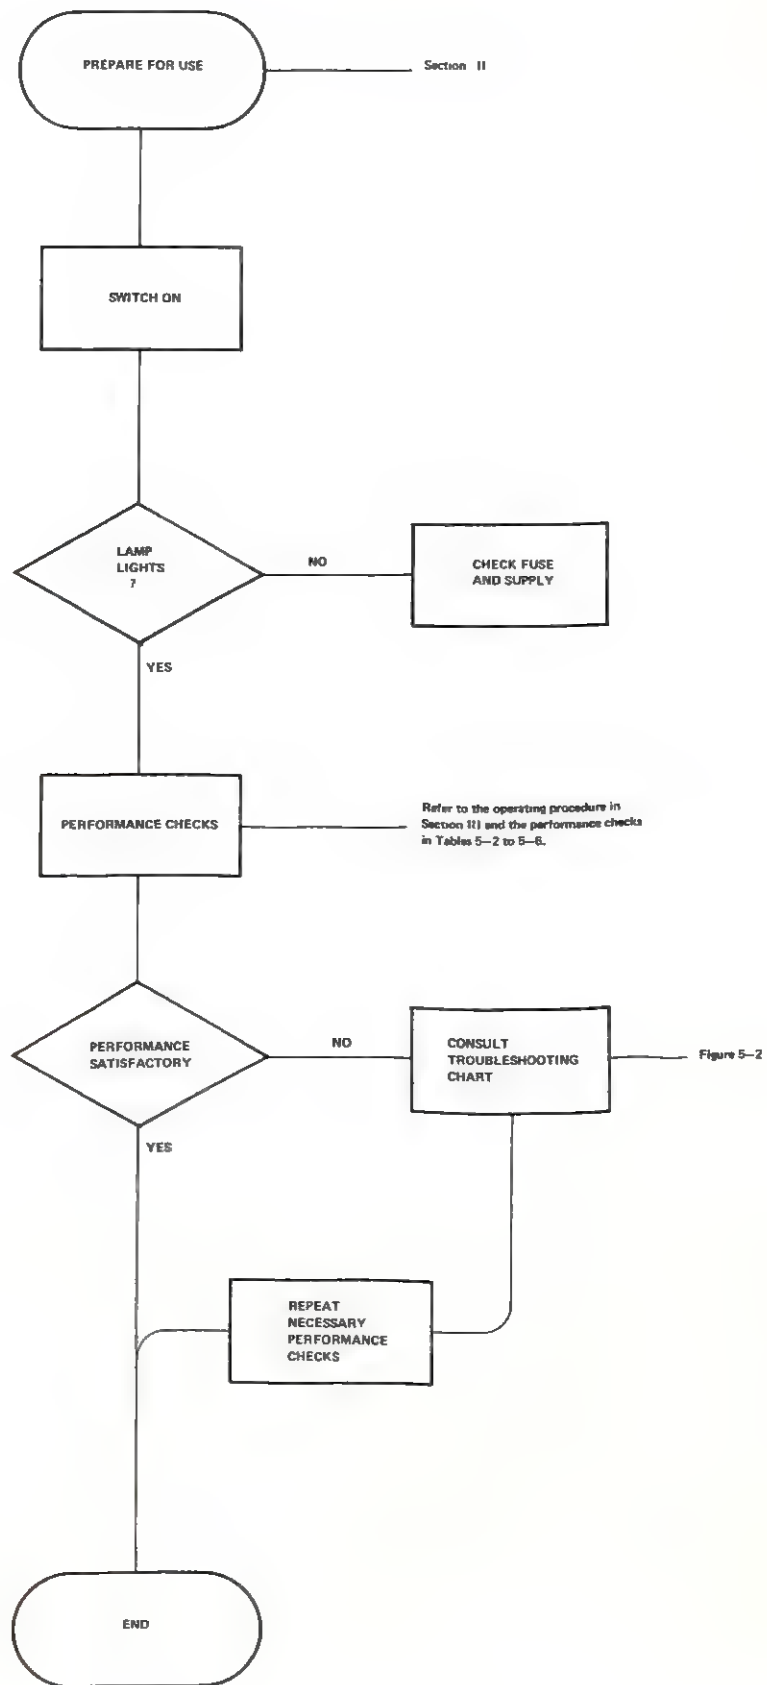


Figure 5-1 Organisation of Tests

Set the 8057A controls as follows:
 CLOCK SEL. switch: INTERNAL
 OUTPUT CONN. switch: NORMAL
 IMPEDANCE: 50

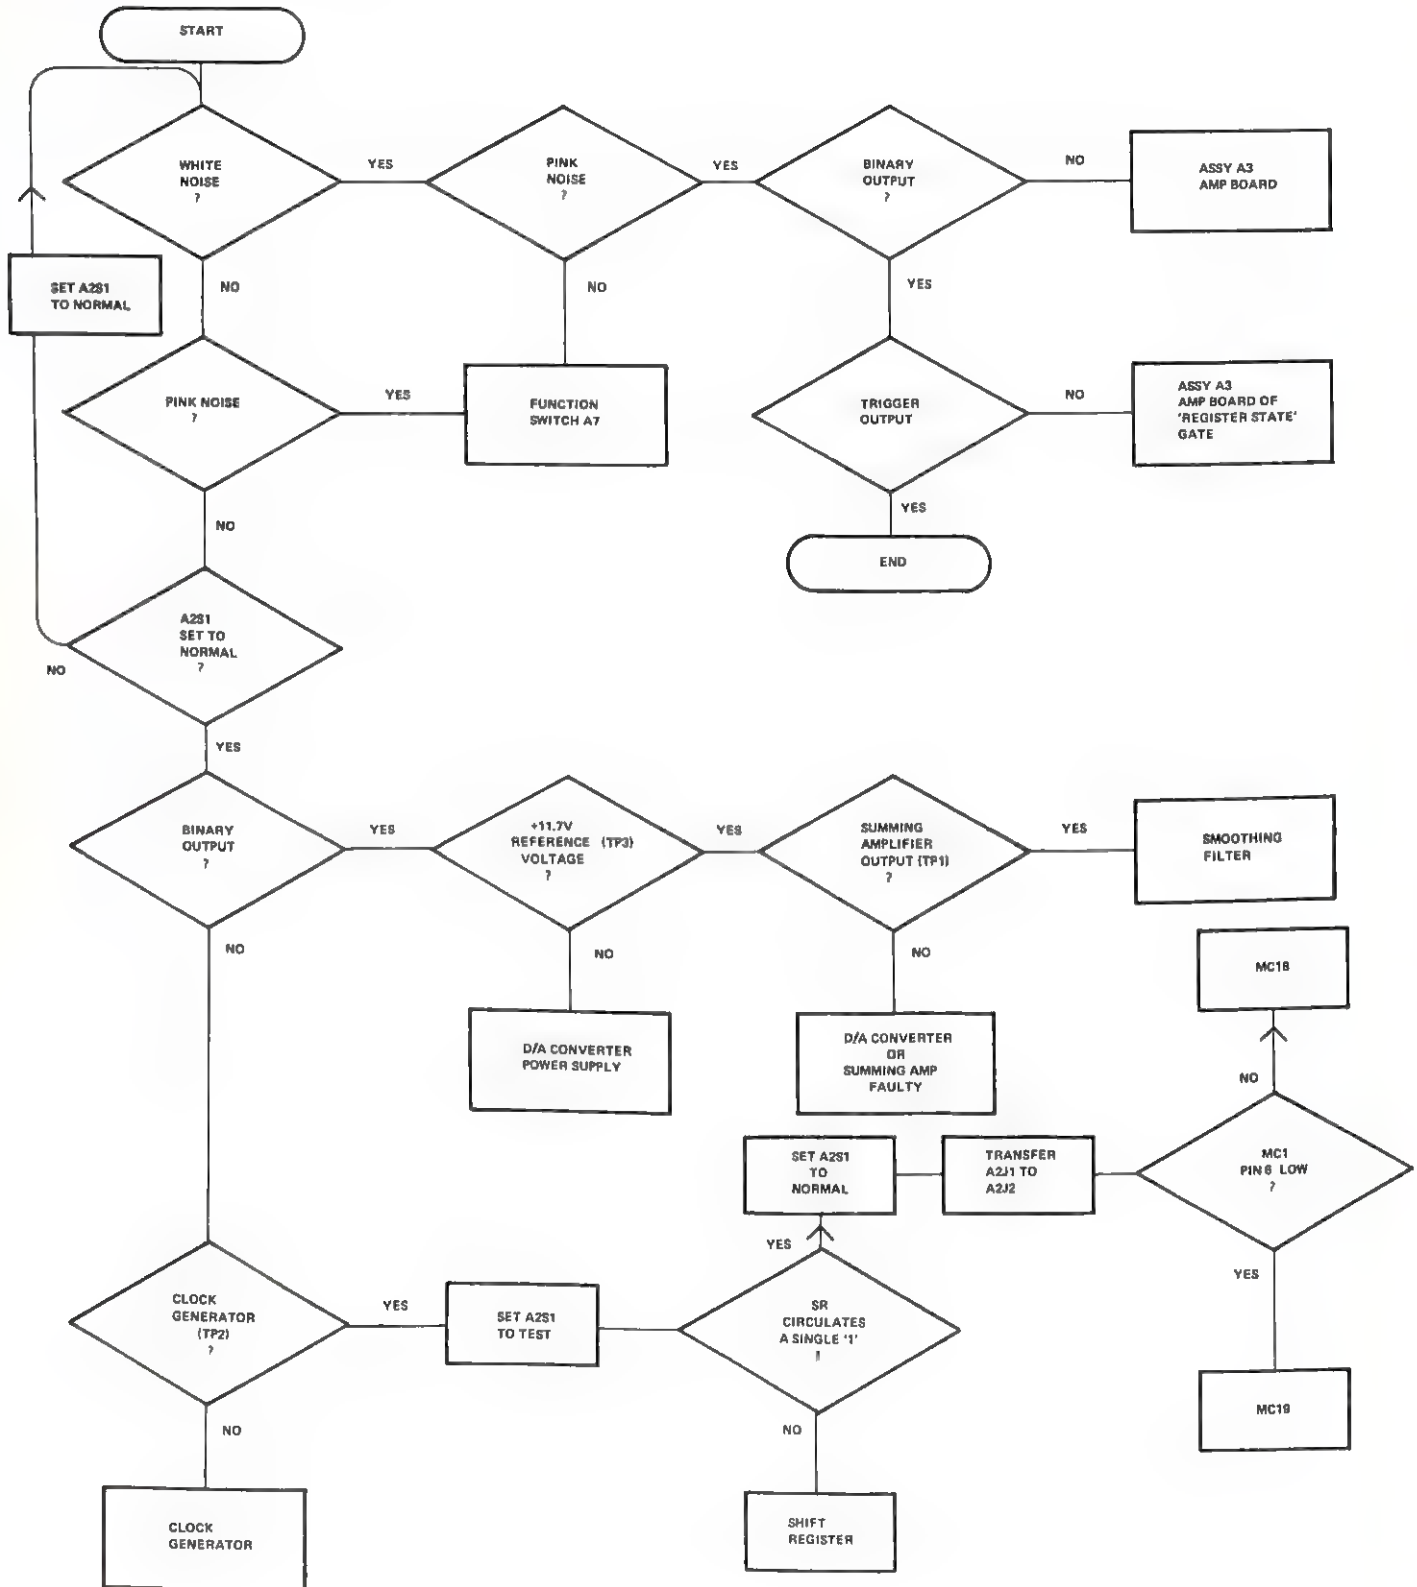


Figure 5-2 Troubleshooting Flow Chart

REPLACEABLE PARTS

6-1 INTRODUCTION

6-2 This section contains information for ordering replacement parts. Table 6-1 lists parts in alpha-numerical order of their reference designators and indicates the description and HP stock number of each part, together with any applicable notes.

6-3 ORDERING INFORMATION

6-4 To order a replacement part, address order of inquiry either to your authorized Hewlett-Packard sales representative or to:

CUSTOMER SERVICE
Hewlett-Packard Company
333 Logue Avenue
Mountain View, California 94040

or, in Western Europe, to:

Hewlett-Packard (Schweiz) SA
Rue du Bois-du-Lan 7
1217 Meyrin 2
Geneva

6-5 Specify the following information for each part:

- a) Model and complete serial number of instrument.
- b) Hewlett-Packard stock number.
- c) Circuit reference designator.
- d) Description.

6-6 To order a part not listed in table 6-1 give a complete description of the part and include its function and location.

REFERENCE DESIGNATORS

A	= assembly	F	= fuse	P	= plug	V	= vacuum tube, neon bulb, photocell, etc.
B	= motor	FL	= filter	Q	= transistor	VR	= voltage regulator
BT	= battery	HR	= heater	R	= resistor	W	= cable
C	= capacitor	J	= jack	RT	= thermistor	X	= socket
CP	= coupler	K	= relay	S	= switch	Y	= crystal
CR	= diode	L	= inductor	T	= transformer		
DL	= delay line	M	= meter	TB	= terminal board		
DS	= lamp	MC	= micro-circuit	TP	= test point		

Table 6-1 Replaceable Parts

REFERENCE DESIGNATOR	H-P PART NUMBER	DESCRIPTION	CIRCUIT DIAGRAM		COMPONENT LAYOUT	REFERENCE DESIGNATOR	H-P PART NUMBER	DESCRIPTION	CIRCUIT DIAGRAM		COMPONENT LAYOUT
			SHEET NUMBER	GRID REFERENCE					SHEET NUMBER	GRID REFERENCE	
A1	08057-66501	RD AY PS				A1	C1	0180-1723	C-F 500UF 50V		
A2	08057-66502	BD AY SHFTRGST				A1	C2	0180-0196	C-F 56UF 15V		
A3	08057-66503	BD AY OUT AMPL				A1	C3	0180-0197	C-F2.2UF 20V		
A4	08057-61901	SW AY STEPATT				A1	C4	0180-0098	C-F 100UF 20V		
A5	08057-61902	SW AY STEPATT				A1	C5	0180-1723	C-F 500UF 50V		
A6	08057-61903	SW AY STEPATT				A1	C6	0180-0196	C-F 56UF 15V		
A7	08057-61904	SW AY PBTN				A1	C7	0180-0197	C-F2.2UF 20V		
C1	0160-2218	C-F .001UF 300V				A1	C8	0180-0098	C-F 100UF 20V		
DS1	2140-0008	LAMP NEON 115V				A1	C9	0180-0237	C-F 500UF 25V		
F1	2110-0201	FUSE .25 FFR				A1	C10	0150-0096	C-F .05UF 100V		
F1	2110-0318	FUSE .125 FFR				A1	C11	0180-0137	C-F 100UF 10V		
J1	1250-0118	CONN RNC BLKWD				A1	C12	0180-0212	C-F 250UF 12V		
J2	1250-0118	SAME AS J 1				A1	C13	0160-2147	C-F .025UF 100V		
J3	1250-0118	SAME AS J 1				A1	C14	0160-2147	C-F .025UF 100V		
J4	1250-0118	SAME AS J 1				A1	CR1	1901-0194	DIO SI 50V .75A		
J5	1250-0118	SAME AS J 1				A1	CR2	1901-0194	DIO SI 50V .75A		
J6	1251-2165	CONN SF RECP				A1	CR3	1901-0194	DIO SI 50V .75A		
J7	1251-2357	CONN PWR AC RECP				A1	CR4	1901-0194	DIO SI 50V .75A		
Q1	775A-0049	P-F 33K5% .25W F				A1	CR5	1902-3107	DIO BKDN 5.76 V		
S1	3101-1235	SW SLIDE OPNT				A1	CR6	1902-0041	DIO BKDN 5.11 V		
S2	3101-1235	SAME AS S 1				A1	CR7	1901-0194	DIO SI 50V .75A		
S3	3101-1234	SW SLIDE OPNT				A1	CR8	1901-0194	DIO SI 50V .75A		
T1	5080-0913	XFMRPWR				A1	CR9	1901-0194	DIO SI 50V .75A		
W1	8120-1349	PWR CORR SET				A1	CR10	1901-0194	DIO SI 50V .75A		
						A1	CR11	1902-3107	DIO BKDN 5.76 V		
						A1	CR12	1902-0041	DIO BKDN 5.11 V		
						A1	CR13	1901-0194	DIO SI 50V .75A		
						A1	CR14	1901-0194	DIO SI 50V .75A		
						A1	CR15	1901-0194	DIO SI 50V .75A		
						A1	CR16	1901-0194	DIO SI 50V .75A		
						A1	CR17	1902-0188	DIO BKDN 4.12 V		
						A1	J1	1251-0213	CONN PC 15 CONT		
						A1	J2	1251-1513	CONN PC 18CONT T		
						A1	Q1	1854-0022	XSTR SI NPN		
						A1	Q2	1854-0072	XSTR 2N3054 SI		
						A1	Q3	1854-0329	XSTR SI NPN		
						A1	Q4	1854-0329	XSTR SI NPN		
						A1	Q5	1854-0307	XSTR SI NPN		
						A1	Q6	1854-0307	XSTR SI NPN		
						A1	Q7	1854-0022	XSTR SI NPN		
						A1	Q8	1854-0072	XSTR 2N3054 SI		
						A1	Q9	1854-0329	XSTR SI NPN		
						A1	Q10	1854-0307	XSTR SI NPN		
						A1	Q11	1854-0307	XSTR SI NPN		
						A1	Q12	1854-0307	XSTR SI NPN		
						A1	Q13	1854-0072	XSTR 2N3054 SI		
						A1	Q14	1854-0329	XSTR SI NPN		
						A1	Q15	1854-0307	XSTR SI NPN		
						A1	Q16	1854-0329	XSTR SI NPN		
						A1	R1	0698-4271	R-F 5.1K5% .125W		
						A1	R2	0698-4271	R-F 5.1K5% .125W		
						A1	R3	0698-4248	R-F 560 5% .125W		
						A1	R4	0727-0001	R-F 1.5 2% .5W		
						A1	R5	0698-4248	R-F 560 5% .125W		
						A1	R6	0698-4290	R-F 33K5% .125W		
						A1	R7	0698-4282	R-F 15K5% .125W		
						A1	R8	0698-4290	R-F 33K5% .125W		
						A1	R9	0698-4253	R-F 910 5% .125W		
						A1	R10	2100-2739	R-VAR 220 2W CER		
						A1	R11	0698-4245	R-F 390 5% .125W		
						A1	R12	0698-4271	R-F 5.1K5% .125W		
						A1	R13	0698-4271	R-F 5.1K5% .125W		
						A1	R14	0698-4248	R-F 560 5% .125W		
						A1	R15	0698-4248	R-F 560 5% .125W		
						A1	R16	0698-4290	R-F 33K5% .125W		
						A1	R17	0698-4282	R-F 15K5% .125W		
						A1	R18	0698-4290	R-F 33K5% .125W		
						A1	R19	0698-4253	R-F 910 5% .125W		
						A1	R20	2100-2739	R-VAR 220 2W CER		
						A1	R21	0698-4245	R-F 390 5% .125W		
						A1	R22	0698-4235	R-F 150 5% .125W		
						A1	R23	0698-4271	R-F 5.1K5% .125W		
						A1	R24	0698-4271	R-F 5.1K5% .125W		
						A1	R25	0727-0001	R-F 1.5 2% .5W		
						A1	R26	0758-0124	R-F 91 5% .125W		
						A1	R27	0698-4644	R-F 20 5% .125W		
						A1	R28	2100-2796	R-VAR 100 .5W		
						A1	R29	0698-4745	R-F 390 5% .125W		
						A1	R30	0698-4258	R-F 1.5K5% .125W		
						A1	R32	0727-0001	R-F 1.5 2% .5W		
						A1	RT1	0837-0015	THMS 500 DISC		

Table 6-1. Replaceable Parts (cont'd)

REFERENCE DESIGNATOR	H-P PART NUMBER	DESCRIPTION	CIRCUIT DIAGRAM		COMPONENT LAYOUT	REFERENCE DESIGNATOR	H-P PART NUMBER	DESCRIPTION	CIRCUIT DIAGRAM		COMPONENT LAYOUT
			SHEET NUMBER	GRID REFERENCE					SHEET NUMBER	GRID REFERENCE	
A2 C2	0180-1746	C-F 15UF 20V				A2 026	1853-0229	XSTR SI PNP			
A2 C3	0140-0157	C-F .01 1857UF				A2 027	1853-0229	XSTR SI PNP			
A2 C4	0160-0153	C-F .01 1UF 200V				A2 028	1853-0229	XSTR SI PNP			
A2 C5	0160-2265	C-F 22PF 500V				A2 029	1853-0229	XSTR SI PNP			
A2 C6	0160-0174	C-F .47UF 25V				A2 030	1853-0229	XSTR SI PNP			
A2 C7	0150-0121	C-F .1UF 50V				A2 034	1853-0000	XSTR SI PNP			
A2 C8	0180-0197	C-F 2.2UF 20V				A2 035	1855-0010	XSTR 2N2646 UJ			
A2 C9	0180-0197	C-F 2.2UF 20V				A2 036	1854-0307	XSTR SI PNP			
A2 C10	0140-0196	C-F 150PF 300V				A2 037	1854-0307	XSTR SI PNP			
A2 C11	0140-0196	C-F 150PF 300V				A2 038	1853-0000	XSTR SI PNP			
A2 CR1	1901-0040	DI0 SI 30V .03A				A2 039	1854-0019	XSTR SI PNP			
A2 CR2	1901-0040	DI0 SI 30V .03A				A2 040	1854-0329	XSTR SI PNP			
A2 CR3	1901-0040	DI0 SI 30V .03A				A2 041	1853-0036	XSTR SI PNP			
A2 CR4	1901-0040	DI0 SI 30V .03A				A2 042	1854-0307	XSTR SI PNP			
A2 CR5	1901-0040	DI0 SI 30V .03A				A2 043	1854-0307	XSTR SI PNP			
A2 CR6	1901-0040	DI0 SI 30V .03A				A2 044	1854-0019	XSTR SI PNP			
A2 CR7	1901-0040	DI0 SI 30V .03A				A2 045	1854-0019	XSTR SI PNP			
A2 CR8	1901-0040	DI0 SI 30V .03A				A2 046	1854-0019	XSTR SI PNP			
A2 CR9	1901-0040	DI0 SI 30V .03A									
A2 CR10	1901-0040	DI0 SI 30V .03A									
A2 CR11	1901-0040	DI0 SI 30V .03A				A2 P1	0698-4257	R-F 1.3K5% .125W			
A2 CR12	1901-0040	DI0 SI 30V .03A				A2 P2	0698-4257	R-F 1.3K5% .125W			
A2 CR13	1901-0040	DI0 SI 30V .03A				A2 P3	0698-4257	R-F 1.3K5% .125W			
A2 CR14	1901-0040	DI0 SI 30V .03A				A2 P4	0698-4257	R-F 1.3K5% .125W			
A2 CR15	1901-0040	DI0 SI 30V .03A				A2 P5	0698-4257	R-F 1.3K5% .125W			
A2 CR16	1901-0040	DI0 SI 30V .03A				A2 P6	0698-4257	R-F 1.3K5% .125W			
A2 CR17	1901-0040	DI0 SI 30V .03A				A2 P7	0698-4257	R-F 1.3K5% .125W			
A2 CR18	1901-0040	DI0 SI 30V .03A				A2 P8	0698-4257	R-F 1.3K5% .125W			
A2 CR19	1901-0040	DI0 SI 30V .03A				A2 P9	0698-4257	R-F 1.3K5% .125W			
A2 CR20	1901-0040	DI0 SI 30V .03A				A2 P10	0698-4257	R-F 1.3K5% .125W			
A2 CR21	1901-0040	DI0 SI 30V .03A				A2 P11	0698-4257	R-F 1.3K5% .125W			
A2 CR22	1901-0040	DI0 SI 30V .03A				A2 P12	0698-4257	R-F 1.3K5% .125W			
A2 CR23	1901-0040	DI0 SI 30V .03A				A2 P13	0698-4257	R-F 1.3K5% .125W			
A2 CR24	1901-0040	DI0 SI 30V .03A				A2 P14	0698-4257	R-F 1.3K5% .125W			
A2 CR25	1901-0040	DI0 SI 30V .03A				A2 P15	0698-4257	R-F 1.3K5% .125W			
A2 CR26	1910-0034	DI0-GE 25V .1A				A2 P16	0698-4257	R-F 1.3K5% .125W			
A2 CR27	1901-0040	DI0 SI 30V .03A				A2 P17	0698-4257	R-F 1.3K5% .125W			
A2 CR28	1901-0040	DI0 SI 30V .03A				A2 P18	0698-4257	R-F 1.3K5% .125W			
A2 CR29	1901-0040	DI0 SI 30V .03A				A2 P19	0698-4257	R-F 1.3K5% .125W			
A2 CR30	1901-0040	DI0 SI 30V .03A				A2 P20	0698-4257	R-F 1.3K5% .125W			
A2 CR31	1901-0040	DI0 SI 30V .03A				A2 P21	0698-4257	R-F 1.3K5% .125W			
A2 CR32	1901-0040	DI0 SI 30V .03A				A2 P22	0698-4257	R-F 1.3K5% .125W			
A2 CR33	1901-0040	DI0 SI 30V .03A				A2 P23	0698-4257	R-F 1.3K5% .125W			
A2 CR34	1901-0040	DI0 SI 30V .03A				A2 P24	0698-4257	R-F 1.3K5% .125W			
A2 CR35	1901-0040	DI0 SI 30V .03A				A2 P25	0698-4257	R-F 1.3K5% .125W			
A2 L1	9140-0111	COIL-CHOKER 3.3MH				A2 R26	0698-4257	R-F 1.3K5% .125W			
A2 MC1	1820-0077	IC 7474N EQUIV				A2 R27	0698-4257	R-F 1.3K5% .125W			
A2 MC2	1820-0077	IC 7474N EQUIV				A2 R28	0698-4257	R-F 1.3K5% .125W			
A2 MC3	1820-0077	IC 7474N EQUIV				A2 R29	0698-4257	R-F 1.3K5% .125W			
A2 MC4	1820-0077	IC 7474N EQUIV				A2 R30	0698-4257	R-F 1.3K5% .125W			
A2 MC5	1820-0077	IC 7474N EQUIV				A2 R31	0757-0484	R-F 61K1% .125W			
A2 MC6	1820-0077	IC 7474N EQUIV				A2 R32	0698-4278	R-F 10K5% .125W			
A2 MC7	1820-0077	IC 7474N EQUIV				A2 R33	0698-4278	R-F 10K5% .125W			
A2 MC8	1820-0077	IC 7474N EQUIV				A2 R34	0698-5797	R-F 296K 1% .125W			
A2 MC9	1820-0077	IC 7474N EQUIV				A2 R35	0698-5796	R-F 196K 1% .125W			
A2 MC10	1820-0077	IC 7474N EQUIV				A2 R36	0698-4278	R-F 10K5% .125W			
A2 MC11	1820-0077	IC 7474N EQUIV				A2 R37	0698-4278	R-F 10K5% .125W			
A2 MC12	1820-0077	IC 7474N EQUIV				A2 R38	0698-5795	R-F 138K 5%			
A2 MC13	1820-0077	IC 7474N EQUIV				A2 R39	0757-0467	R-F 121K1% .125W			
A2 MC14	1820-0077	IC 7474N EQUIV				A2 R40	0698-4278	R-F 10K5% .125W			
A2 MC15	1820-0077	IC 7474N EQUIV				A2 R41	0698-4278	R-F 10K5% .125W			
A2 MC16	1820-0077	IC 7474N EQUIV				A2 R42	0757-0469	R-F 15K1% .125W			
A2 MC17	1820-0063	IC 7474N EQUIV				A2 R43	0757-0472	R-F 20K1% .125W			
A2 MC18	1820-0054	IC 7474N EQUIV				A2 R44	0698-4278	R-F 10K5% .125W			
A2 MC19	1820-0054	IC 7474N EQUIV				A2 R45	0757-0467	R-F 121K1% .125W			
A2 Q1	1853-0229	XSTR SI PNP				A2 R46	0698-4278	R-F 10K5% .125W			
A2 Q2	1853-0229	XSTR SI PNP				A2 R47	0698-4278	R-F 10K5% .125W			
A2 Q3	1853-0229	XSTR SI PNP				A2 R48	0698-5794	R-F 52.6K 5%			
A2 Q4	1853-0229	XSTR SI PNP				A2 R49	0698-5793	R-F 31.1K 5%			
A2 Q5	1853-0229	XSTR SI PNP				A2 R50	0698-4282	R-F 15K5% .125W			
A2 Q6	1853-0229	XSTR SI PNP				A2 R51	0698-4284	R-F 18K5% .125W			
A2 Q7	1853-0229	XSTR SI PNP				A2 R52	0698-4888	R-F 21.3K 5%			
A2 Q8	1853-0229	XSTR SI PNP				A2 R53	0698-6880	R-F 16K 5% .125W			
A2 Q9	1853-0229	XSTR SI PNP				A2 R54	0698-4288	R-F 27K5% .125W			
A2 Q10	1853-0229	XSTR SI PNP				A2 R55	0698-6877	R-F 12.9K 5%			
A2 Q11	1853-0229	XSTR SI PNP				A2 R56	0698-5780	R-F 11.1K 5%			
A2 Q12	1853-0229	XSTR SI PNP				A2 R57	0698-6871	R-F 10K 5% .125W			
A2 Q13	1853-0229	XSTR SI PNP				A2 R58	0698-6871	R-F 10K 5% .125W			
A2 Q14	1853-0229	XSTR SI PNP				A2 R59	0698-5780	R-F 11.1K 5%			
A2 Q15	1853-0229	XSTR SI PNP				A2 R60	0698-6877	R-F 12.9K 5%			
A2 Q16	1853-0229	XSTR SI PNP				A2 R61	0698-4288	R-F 27K5% .125W			
A2 Q17	1853-0229	XSTR SI PNP				A2 R62	0698-6880	R-F 16K 5% .125W			
A2 Q18	1853-0229	XSTR SI PNP				A2 R63	0698-4284	R-F 18K5% .125W			
A2 Q19	1853-0229	XSTR SI PNP				A2 R64	0698-6888	R-F 21.3K 5%			
A2 Q20	1853-0229	XSTR SI PNP				A2 R65	0698-4282	R-F 15K5% .125W			
A2 Q21	1853-0229	XSTR SI PNP				A2 R66	0698-5793	R-F 31.1K 5%			
A2 Q22	1853-0229	XSTR SI PNP				A2 R67	0698-4278	R-F 10K5% .125W			
A2 Q23	1853-0229	XSTR SI PNP				A2 R68	0698-5794	R-F 52.6K 5%			
A2 Q24	1853-0229	XSTR SI PNP				A2 R69	0698-4278	R-F 10K5% .125W			
A2 Q25	1853-0229	XSTR SI PNP				A2 R70	0757-0467	R-F 121K1% .125W			

Table 6-1. Replaceable Parts (cont'd)

REFERENCE DESIGNATOR	H-P PART NUMBER	DESCRIPTION	CIRCUIT DIAGRAM		COMPONENT LAYOUT
			SHEET NUMBER	GRID REFERENCE	
A2	R71	0698-4278	P-F	10K57	.125W
A2	R72	0757-0472	P-F	200K17	.125W
A2	R73	0757-0469	P-F	150K17	.125W
A2	R74	0698-4278	P-F	10K57	.125W
A2	R75	0698-4278	P-F	10K57	.125W
A2	R76	0757-0467	P-F	121K17	.125W
A2	R77	0698-5799	P-F	138K.5R	
A2	R78	0698-4278	P-F	10K57	.125W
A2	R79	0698-4278	P-F	10K57	.125W
A2	R80	0698-5796	P-F	186K 1R	.125
A2	R81	0698-5797	P-F	296K 17	.125
A2	R82	0698-4278	P-F	10K57	.125W
A2	R83	0698-4278	P-F	10K57	.125W
A2	R84	0757-0494	P-F	619K17	.125W
A2	R85	0757-0415	P-F	430 27	.125W
A2	R92	0698-4254	P-F	1K57	.125W F
A2	R93	0698-4271	P-F	5.1K57	.125W
A2	R94	0698-4258	P-F	1.5K57	.125W
A2	R95	0698-4235	P-F	150 57	.125W
A2	R96	0758-0124	P-F	51 57	.125W
A2	R97	0698-4259	P-F	1.1K57	.125W
A2	R98	0698-4254	P-F	1K57	.125W F
A2	R99	0698-4271	P-F	5.1K57	.125W
A2	R100	0698-4265	P-F	3K57	.125W F
A2	R101	0698-4242	P-F	300 57	.125W
A2	R102	0757-0437	P-F	4.75K17	
A2	R103	0757-0438	P-F	5.11K17	
A2	R104	0698-4264	P-F	2.7K57	.125W
A2	R105	0757-0415	P-F	430 27	.125W
A2	R106	0757-0430	P-F	2.21K17	
A2	R107	0698-4258	P-F	1.5K57	.125W
A2	R108	0698-4247	P-F	510 57	.125W
A2	R109	0757-0407	P-F	200 17	.125W
A2	R110	0698-4252	P-F	820 57	.125W
A2	R111	0698-4269	P-F	4.3K57	.125W
A2	R112	0698-4269	P-F	4.3K57	.125W
A2	R113	0698-4264	P-F	2.7K57	.125W
A2	R114	0698-4254	P-F	1K57	.125W F
A2	R115	0757-0430	P-F	2.21K17	
A2	R116	0757-0273	P-F	3.01K17	
A2	R117	0757-0915	P-F	430 27	.125W
A2	R119	0757-0824	P-F	2K17	.4W MF
A2	R120	0757-0408	P-F	243 17	.125W
A2	R122	0698-4254	P-F	1K57	.125W F
A2	R123	0698-4254	P-F	1K57	.125W F
A2	R124	0698-4259	P-F	1.6K57	.125W
A2	R125	0698-4254	P-F	1K57	.125W F
A2	R126	2100-2777	P-F	VAR 1K	.5W
A2	S1	08057-21901	SW	SLTD	

Table 6-1. Replaceable Parts (cont'd)

REFERENCE DESIGNATOR	H-P PART NUMBER	DESCRIPTION	CIRCUIT DIAGRAM		COMPONENT LAYOUT
			SHEET NUMBER	GRID REFERENCE	
A3 C1	0160-0153	C-F .001UF 200V			
A3 C2	0160-2257	C-F .10PF 50V			
A3 C3	0150-1743	C-F .1UF 35V			
A3 C4	0160-2228	C-F .0027UF 300V			
A3 C5	0160-2210	C-F .47PF 300V			
A3 C6	0160-2257	C-F .10PF 50V			
A3 C7	0160-0153	C-F .001UF 200V			
A3 C8	0180-1743	C-F .1UF 35V			
A3 C9	0150-0121	C-F .1UF 50V			
A3 C10	0150-0121	C-F .1UF 50V			
A3 C12	0180-0159	C-F .22UF 10V			
A3 C13	0180-0159	C-F .22UF 10V			
A3 C14	0140-0193	C-F .82PF 300V			
A3 C15	0160-2218	C-F .001UF 300V			
A3 C16	0140-0157	C-F .00187UF			
A3 C17	0160-2127	C-F .0046UF 300V			
A3 C18	0160-2151	C-F .011UF 200V			
A3 C19	0160-3385	C-F .03UF 150V			
A3 C20	0160-3384	C-F .072UF 160V			
A3 C21	0160-2194	C-F .1UF 200V			
A3 C22	0160-3383	C-F .43UF 63V			
A3 C23	0160-0542	C-F .1UF 50V			
A3 C24	0150-0121	C-F .1UF 50V			
A3 C25	0160-0174	C-F .47UF 25V			
A3 C27	0180-0107	C-F .2UF 20V			
A3 C28	0180-0197	C-F .2UF 20V			
A3 C29	0150-0093	C-F .01UF 100V			
A3 C31	1901-0040	DIO SI 30V .03A			
A3 C42	1901-0040	DIO SI 30V .03A			
A3 C43	1901-0040	DIO SI 30V .03A			
A3 C44	1901-0040	DIO SI 30V .03A			
A3 J1	1251-0131	C744N TEST POINT			
A3 Q1	1854-0221	XSTR SI NPN			
A3 Q3	1854-0307	XSTR SI NPN			
A3 Q4	1854-0307	XSTR SI NPN			
A3 Q5	1853-0036	XSTR SI PNP			
A3 Q6	1854-0329	XSTR SI NPN			
A3 Q7	1854-0329	XSTR SI NPN			
A3 Q8	1853-0036	XSTR SI PNP			
A3 Q9	1854-0221	XSTR SI NPN			
A3 Q11	1854-0307	XSTR SI NPN			
A3 Q12	1854-0307	XSTR SI NPN			
A3 Q13	1853-0036	XSTR SI PNP			
A3 Q14	1854-0329	XSTR SI NPN			
A3 Q15	1854-0329	XSTR SI NPN			
A3 Q16	1853-0036	XSTR SI PNP			
A3 Q17	1853-0027	XSTR SI PNP			
A3 Q18	1854-0090	XSTR SI NPN			
A3 Q19	1854-0019	XSTR SI NPN			
A3 Q20	1854-0019	XSTR SI NPN			
A3 Q21	1853-0036	XSTR SI PNP			
A3 Q22	1853-0036	XSTR SI PNP			
A3 Q23	1853-0090	XSTR SI PNP			
A3 Q24	1854-0307	XSTR SI NPN			
A3 Q25	1853-0090	XSTR SI PNP			
A3 R1	0698-4252	R-F 820 5% .125W			
A3 R2	2100-2787	R-VAR 220 .5W			
A3 R3	0698-0095	R-F 2.61K 1% .125W			
A3 R4	0757-0467	R-F 121K 1% .125W			
A3 R5	0698-4286	R-F 22K 5% .125W			
A3 R6	0698-4306	R-F 150K 5% .125W			
A3 R7	0757-0467	R-F 121K 1% .125W			
A3 R8	0698-4252	R-F 820 5% .125W			
A3 R10	0698-4305	R-F 130K 5% .125W			
A3 R11	0698-4289	R-F 30K 5% .125W			
A3 R12	0757-0283	R-F 2K 1% .125W F			
A3 R13	0683-3345	R-F 330K 5% .25W			
A3 R14	0698-4289	R-F 30K 5% .125W			
A3 R15	0698-4263	R-F 2.4K 5% .125W			
A3 R16	0698-4263	R-F 2.4K 5% .125W			
A3 R17	0698-4287	R-F 10 5% .125W			
A3 R18	0698-4287	R-F 10 5% .125W			
A3 R19	0757-0283	R-F 2K 1% .125W F			
A3 R20	0757-0283	R-F 1K 1% .125W F			
A3 R23	0698-4252	R-F 820 5% .125W			
A3 R24	0698-4304	R-F 120K 5% .125W			
A3 R25	0698-4286	R-F 22K 5% .125W			
A3 R26	0698-4306	R-F 150K 5% .125W			
A3 R27	0698-4305	R-F 130K 5% .125W			
A3 R29	0698-4269	R-F 4.3K 5% .125W			
A3 R30	0698-4305	R-F 130K 5% .125W			
A3 R31	0698-4289	R-F 30K 5% .125W			
A3 R32	0683-3345	R-F 330K 5% .25W			
A3 R33	0698-4289	R-F 30K 5% .125W			
A3 R34	0698-4263	R-F 2.4K 5% .125W			
A3 R35	0698-4263	R-F 2.4K 5% .125W			
A3 R36	0698-4231	R-F 91 5% .125W			
A3 R37	0758-0124	R-F 51 5% .125W			
A3 R38	0758-0124	R-F 51 5% .125W			
A3 R39	0698-4231	R-F 91 5% .125W			
A3 R40	0757-0401	R-F 100 1% .125W			
A3 R42	0757-0401	R-F 100 1% .125W			
A3 R43	0698-4097	R-F 94.8 1% .125W			
A3 R44	0757-0411	R-F 332 1% .125W			
A3 R45	0698-4229	R-F 870 .5%			
A3 R46	0757-0401	R-F 2.21K 1%			
A3 R47	0698-7294	R-F 5.55K 1%			
A3 R48	0698-7290	R-F 13.8K 1%			
A3 R49	0757-0123	R-F 34.8K 1%			
A3 R50	0698-7291	R-F 89.6K 1%			
A3 R51	0698-7293	R-F 251K 1% .25W			
A3 R52	0757-0121	R-F 258K 1% .25W			
A3 R53	0698-4248	R-F 560 5% .125W			
A3 R54	0757-0273	R-F 3.01K 1%			
A3 R55	0757-0436	R-F 4.32K 1%			
A3 R56	0698-4258	R-F 1.5K 5% .125W			
A3 R57	0698-4265	R-F 3K 5% .125W F			
A3 R60	0757-0407	R-F 200 1% .125W			
A3 R61	0757-0407	R-F 200 1% .125W			
A3 R62	0757-0421	R-F 825 1% .125W			
A3 R63	0698-4256	R-F 1.2K 5% .125W			
A3 R64	0698-4256	R-F 1.2K 5% .125W			
A3 R65	2100-2787	R-VAR 220 .5W			
A3 R66	0757-0121	R-F 258K 1% .25W			
A3 R67	0757-0429	R-F 1.82K 1%			
A3 R68	2100-2741	R-VAR 470 2W CER			
A3 R69	0698-4264	R-F 2.7K 5% .125W			
A3 R70	2100-2791	R-VAR 100K .5W			
A3 R71	0698-4234	R-F 130 5% .125W			
A3 R72	0757-0424	R-F 1.1K 1% .125W			
A3 R73	0757-0435	R-F 3.92K 1%			
A3 R74	0698-4263	R-F 2.4K 5% .125W			
A3 R75	0698-4235	R-F 150 5% .125W			
A3 R76	0698-4260	R-F 1.8K 5% .125W			
REFERENCE DESIGNATOR	H-P PART NUMBER	DESCRIPTION	CIRCUIT DIAGRAM		COMPONENT LAYOUT
			SHEET NUMBER	GRID REFERENCE	
A4 C1	0160-2144	C-F .0037UF 1KV			
A4 R1	0698-4190	R-F 50 .25W			
A4 R2	0698-4580	R-F 25K .5% .125W			
A4 R3	0698-4190	R-F 50 .25W			
A4 R4	0698-6232	R-F 53.3 .5%			
A4 R5	0698-6230	R-F 790 .5%			
A4 R6	0698-6232	R-F 53.3 .5%			
A4 R7	0698-6233	R-F 61.11 .5%			
A4 R9	0698-6276	R-F 247.5 .5%			
A4 R9	0698-6233	R-F 61.11 .5%			
A4 R10	0698-6235	R-F 96.25 .5%			
A4 R11	0698-6227	R-F 71.16 .5%			
A4 R12	0698-6235	R-F 96.25 .5%			
A4 S1	3100-0518	SW-ROT 45EC11P05			

Table 6-1. Replaceable Parts (cont'd)

REFERENCE DESIGNATOR	H-P PART NUMBER	DESCRIPTION	CIRCUIT DIAGRAM		COMPONENT LAYOUT
			SHEET NUMBER	GRID REFERENCE	
A5 R1	0757-0284	R-F 150 1% .125W			
A5 R2	0727-0017	R-F 37.35 .5%			
A5 R3	0757-0284	R-F 150 1% .125W			
A5 R4	0698-6236	R-F 292.4 .5%			
A5 R5	0698-6234	R-F 17.61 .5%			
A5 R6	0698-6236	R-F 292.4 .5%			
A5 R7	0698-6237	R-F 436.2 .5%			
A5 R8	0698-6231	R-F 11.61 .5%			
A5 R9	0698-6237	R-F 436.2 .5%			
A5 R10	0698-6229	R-F 870 .5%			
A5 R11	0727-0005	R-F 5.77 .5%			
A5 R12	0698-6229	R-F 870 .5%			
A5 S1	3100-0517	SW-PDT 5SEC10POS			

REFERENCE DESIGNATOR	H-P PART NUMBER	DESCRIPTION	CIRCUIT DIAGRAM		COMPONENT LAYOUT
			SHEET NUMBER	GRID REFERENCE	
A6 C1	0160-2144	C-F .0033UF 1KV			
A6 R1	0698-7292	R-F 1.45K .5%			
A6 R2	0683-0685	R-F 6.8 5% .25W			
A6 R3	0727-0446	R-F 7 1% .5W CF			
A6 R4	0698-7292	R-F 1.45K .5%			
A6 R5	0698-7289	R-F 2.91K .5%			
A6 R6	0811-2108	R-F 1.722 .5%			
A6 R7	0698-7289	R-F 2.91K .5%			
A6 R8	0698-4442	R-F 4.42K 1%			
A6 R9	0811-2738	R-F 1.15 .5%			
A6 R10	0698-4442	R-F 4.42K 1%			
A6 R11	0698-6206	R-F 8.76K 1%			
A6 R12	0811-2738	R-F 1.15 .5%			
A6 R13	0811-2738	R-F 1.15 .5%			
A6 R14	0698-6206	R-F 8.76K 1%			
A6 S1	3100-0517	SW-PDT 5SEC10POS			

REFERENCE DESIGNATOR	H-P PART NUMBER	DESCRIPTION	CIRCUIT DIAGRAM		COMPONENT LAYOUT
			SHEET NUMBER	GRID REFERENCE	
A7 R1	0698-4265	R-F 3K5% .125W F			
A7 R2	0757-1016	R-F 550 .25% .5W			
A7 S1	3101-0518	SW P-BTN 7SECT			

7-1 INTRODUCTION

7-2 This section contains the block, circuit and component location diagrams necessary for servicing the noise generator. A summary of symbols and references appears in Figure 7-1 and a summary of logic symbols and associated truth tables in Figure 7-2.


7-3 The noise generator consists of seven assemblies (A1 to A7) mounted in a frame. Components mounted on the assemblies are prefixed by the appropriate assembly number, thus A2CR1 is a diode mounted on A2. Components mounted directly on the frame

have not prefix. Integrated circuit packages containing more than one functional element are treated separately, each element being identified by a flip-flop designation e. g., MC1 consists of two flip-flops: FF1 and FF2.

7-4 Connections between assemblies are made as follows:


1. Directly by means of flying leads or flying screened leads. These are identified by a colour code.
2. Edge connector sockets mounted on the assemblies. Connections between these sockets are made by printed circuitry.

Figure 7-1. General Symbols and References.

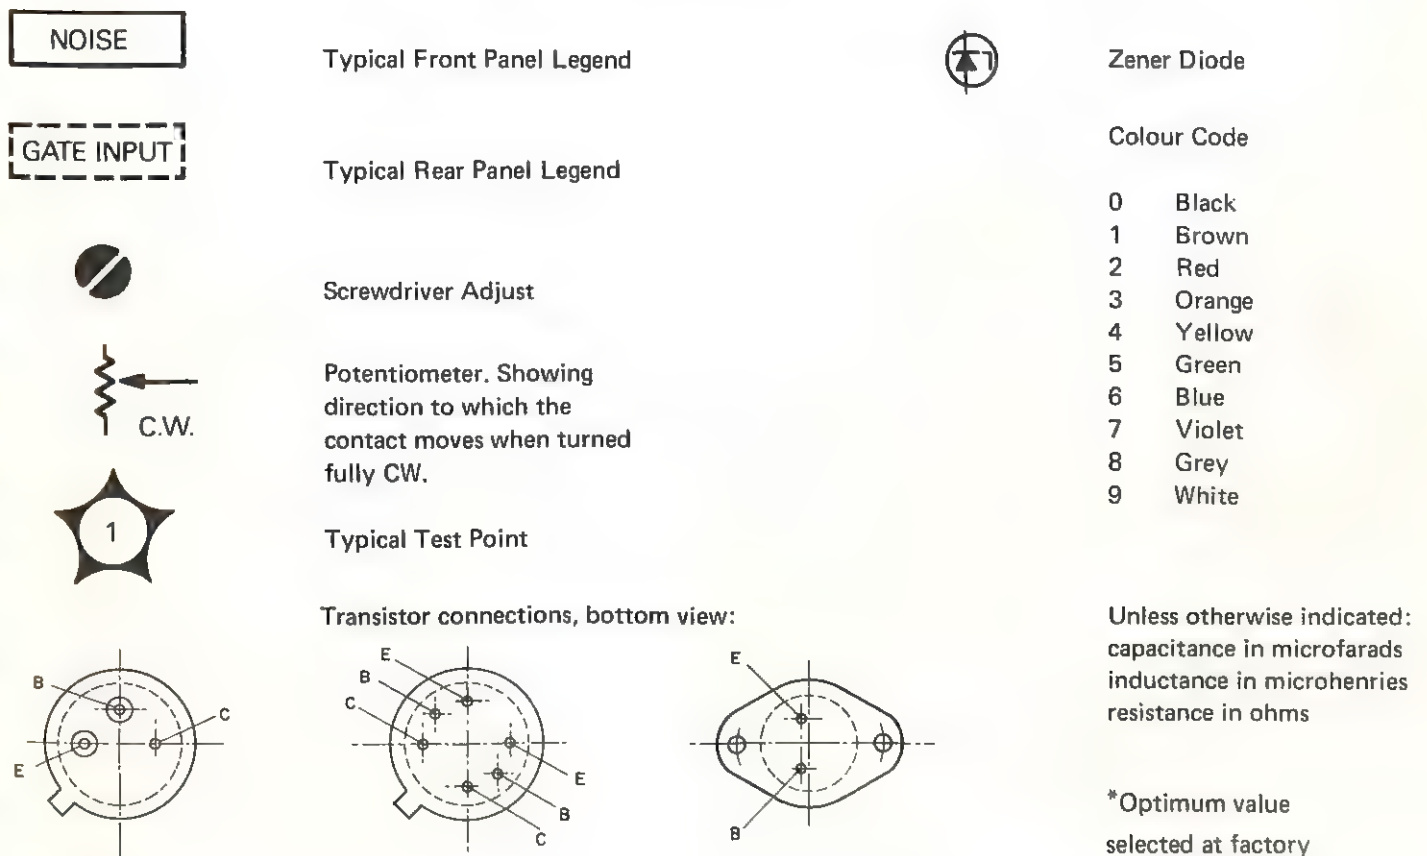


1820-0054

QUADRUPLER 2-INPUT POSITIVE NAND GATE

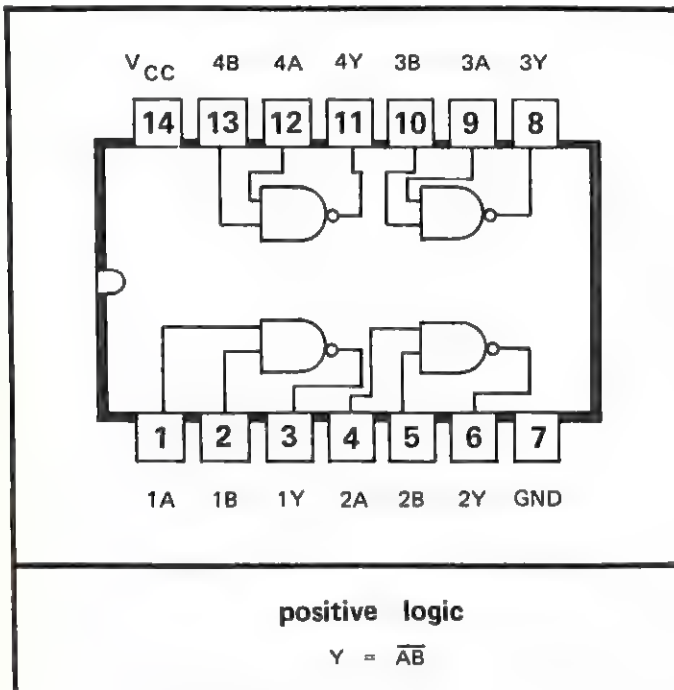


1820-0063

DUAL EXCLUSIVE OR GATE

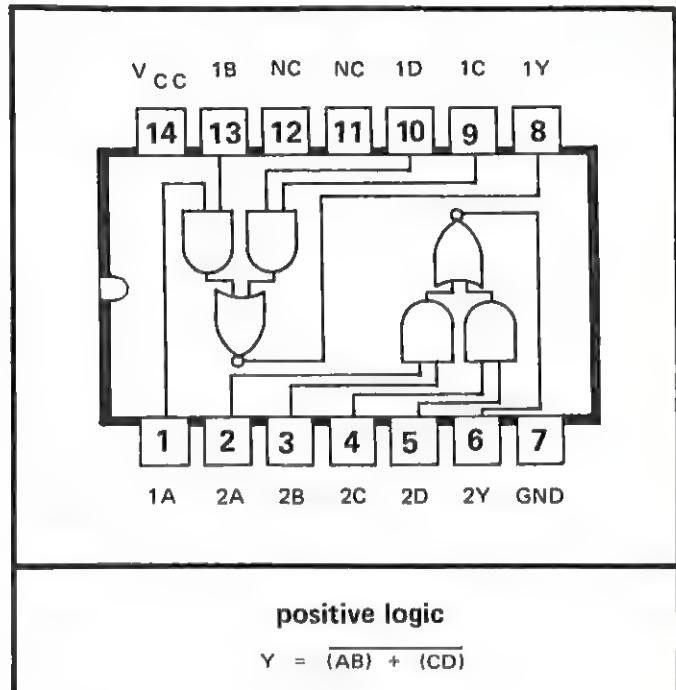

1820-0077

DUAL D-TYPE EDGE-TRIGGERED FLIP-FLOP

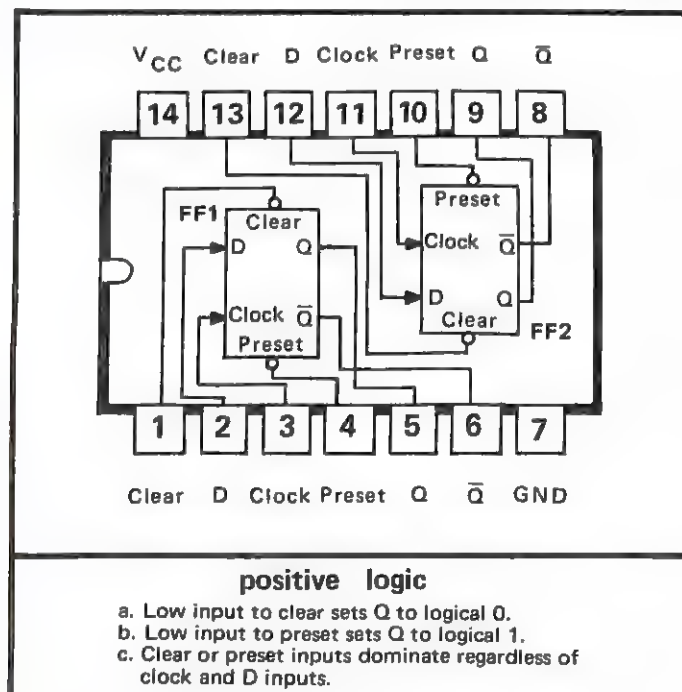

TRUTH TABLE (Each Flip-Flop)

t_n	t_{n+1}	
INPUT D	OUTPUT Q	OUTPUT \bar{Q}
0	0	1
1	1	0

NOTES: 1. t_n = bit time before clock pulse2. t_{n+1} = bit time after clock pulse

Figure 7-2 Microcircuit Packages

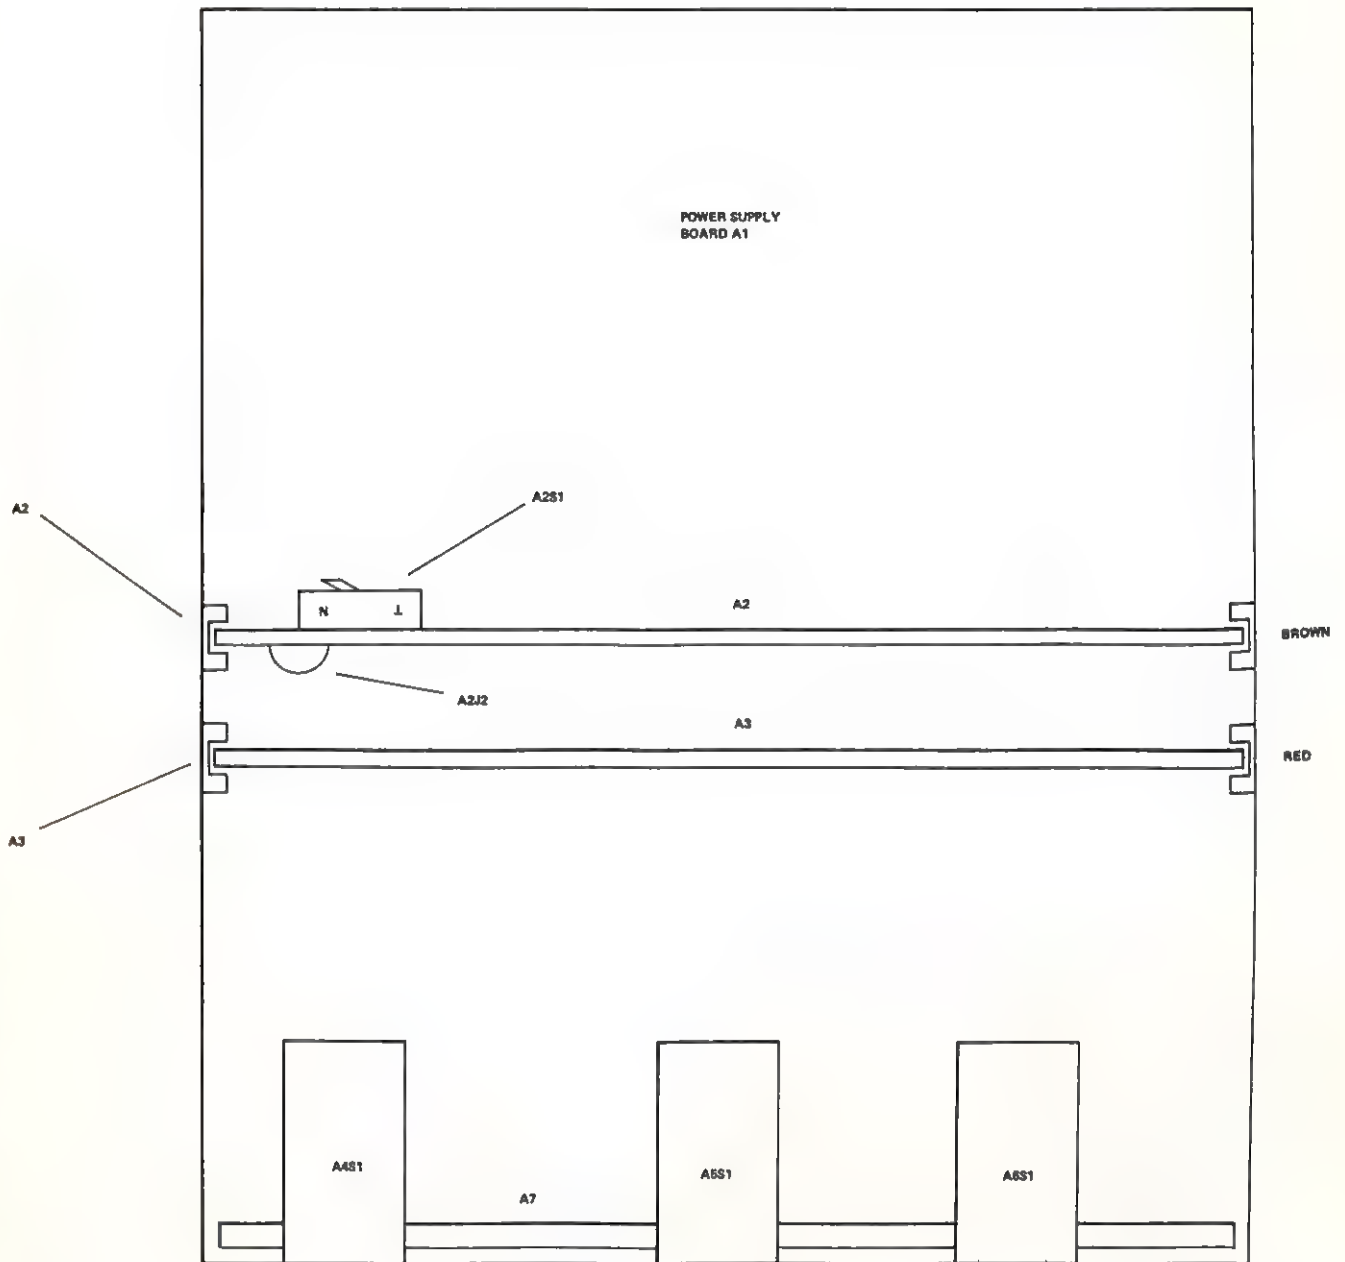


Figure 7-3 Assembly Location



Figure 7–4 Assembly 2 Component Layout

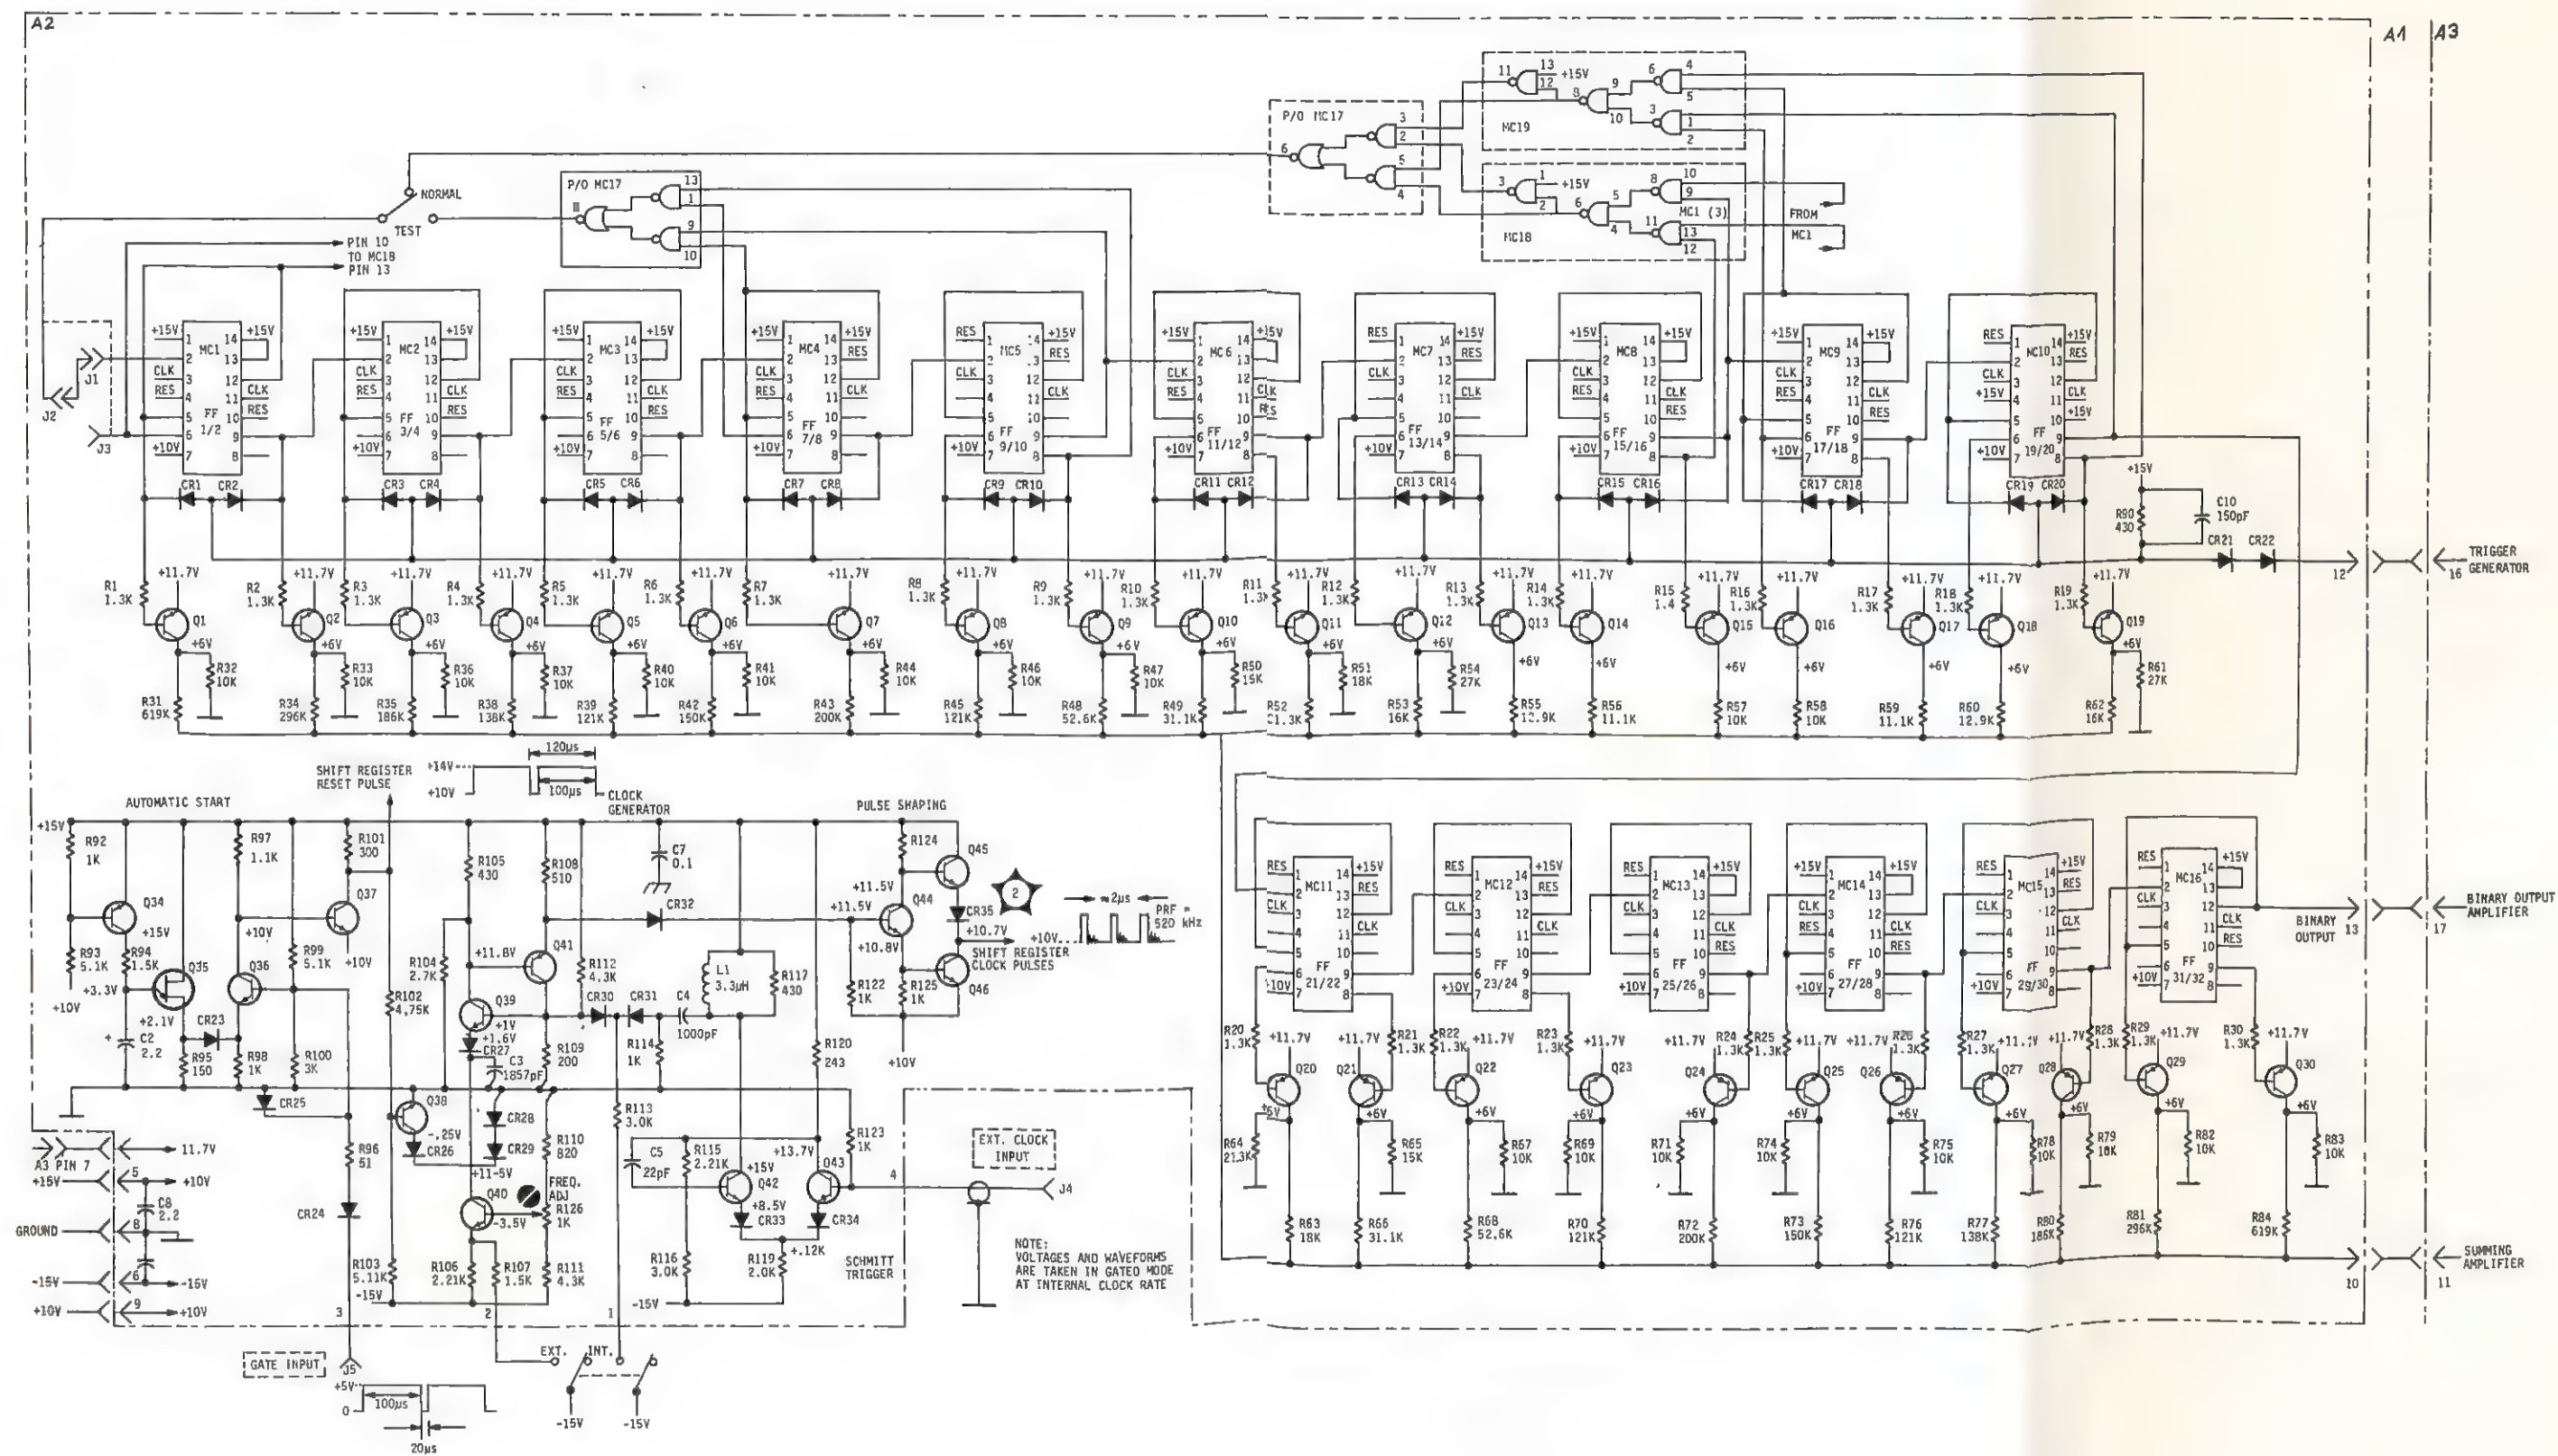


Figure 7-5. Assembly 2 Circuit Diagram



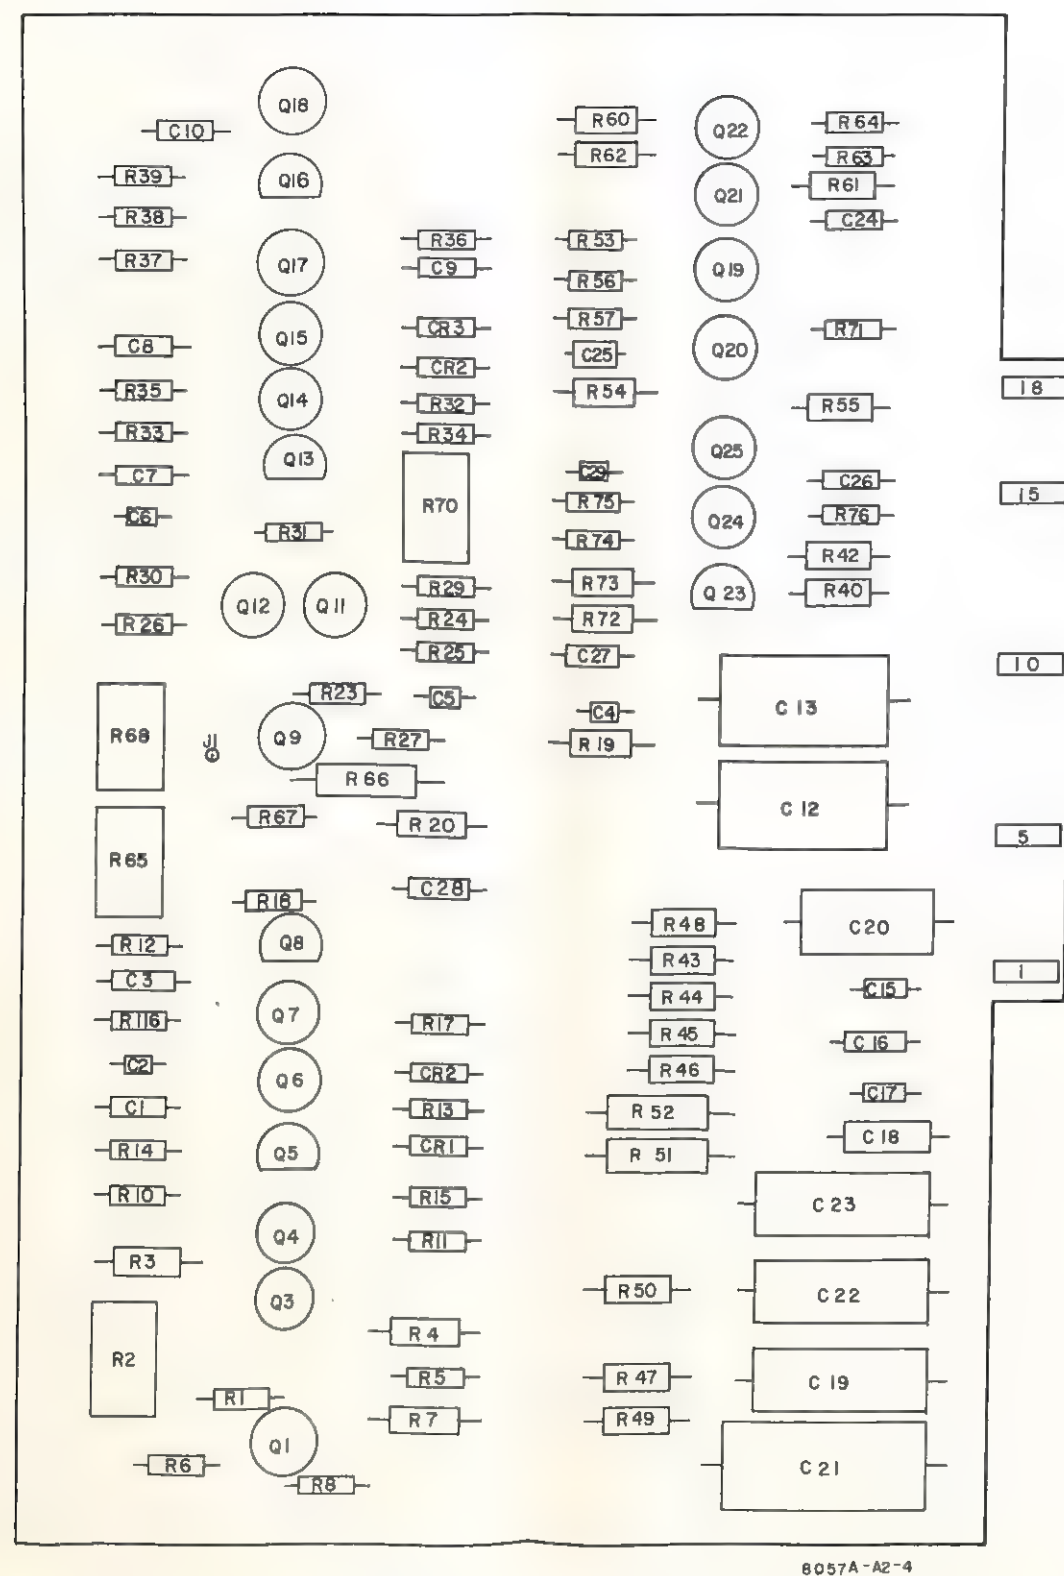


Figure 7-6 Assembly 3 Component Layout and Waveforms

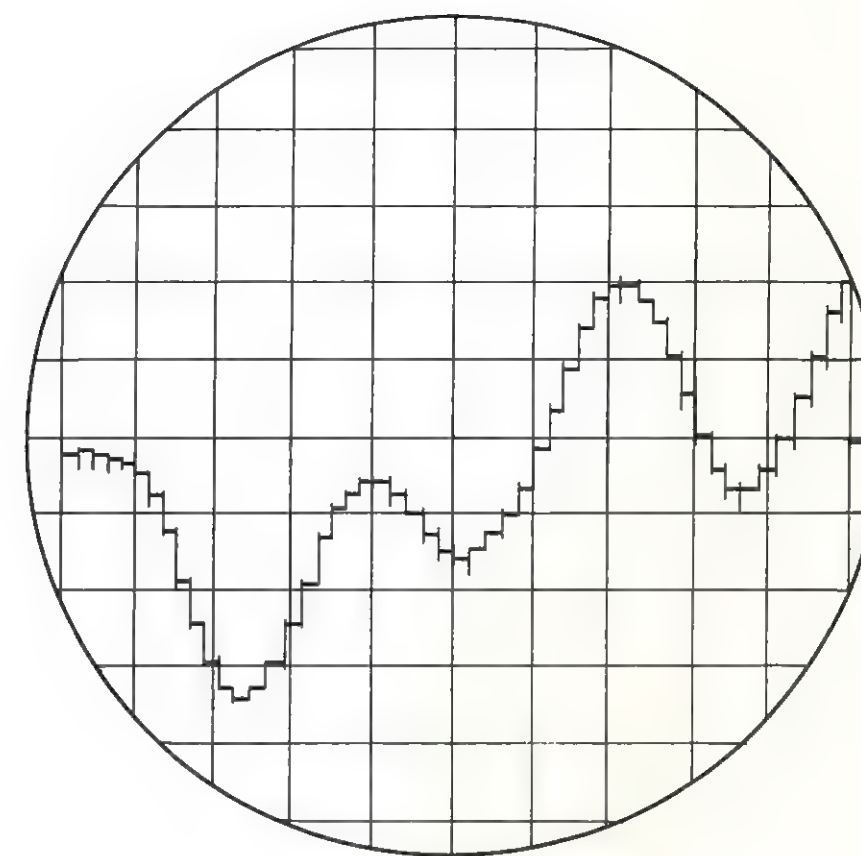

Summing amplifier output (TP1)

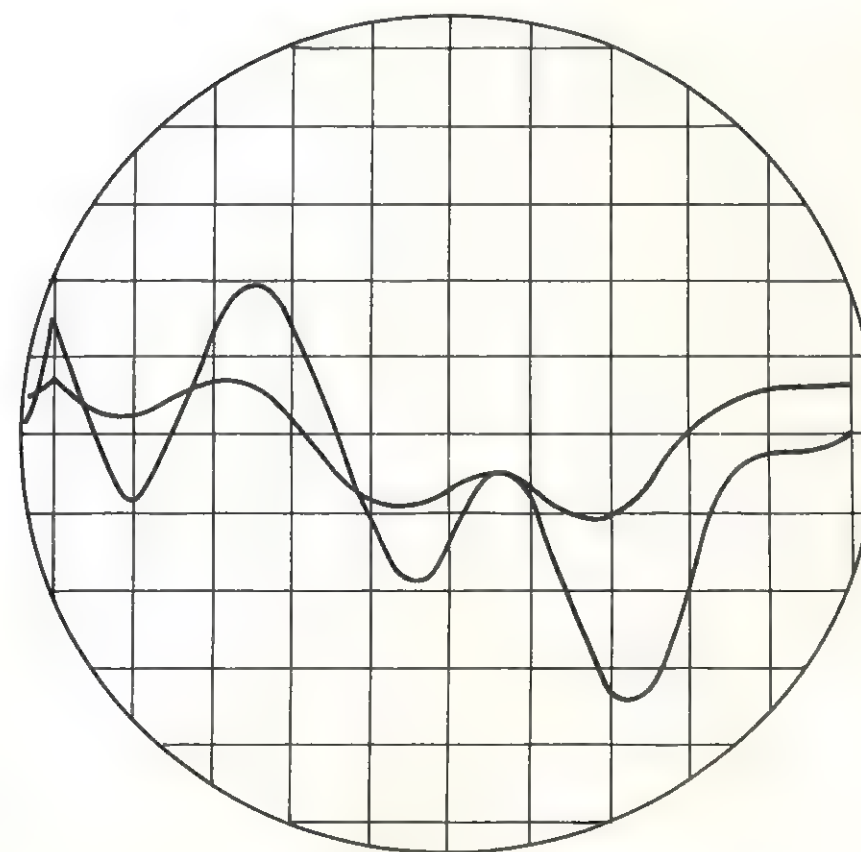

Smoothing filter output (pin 13)

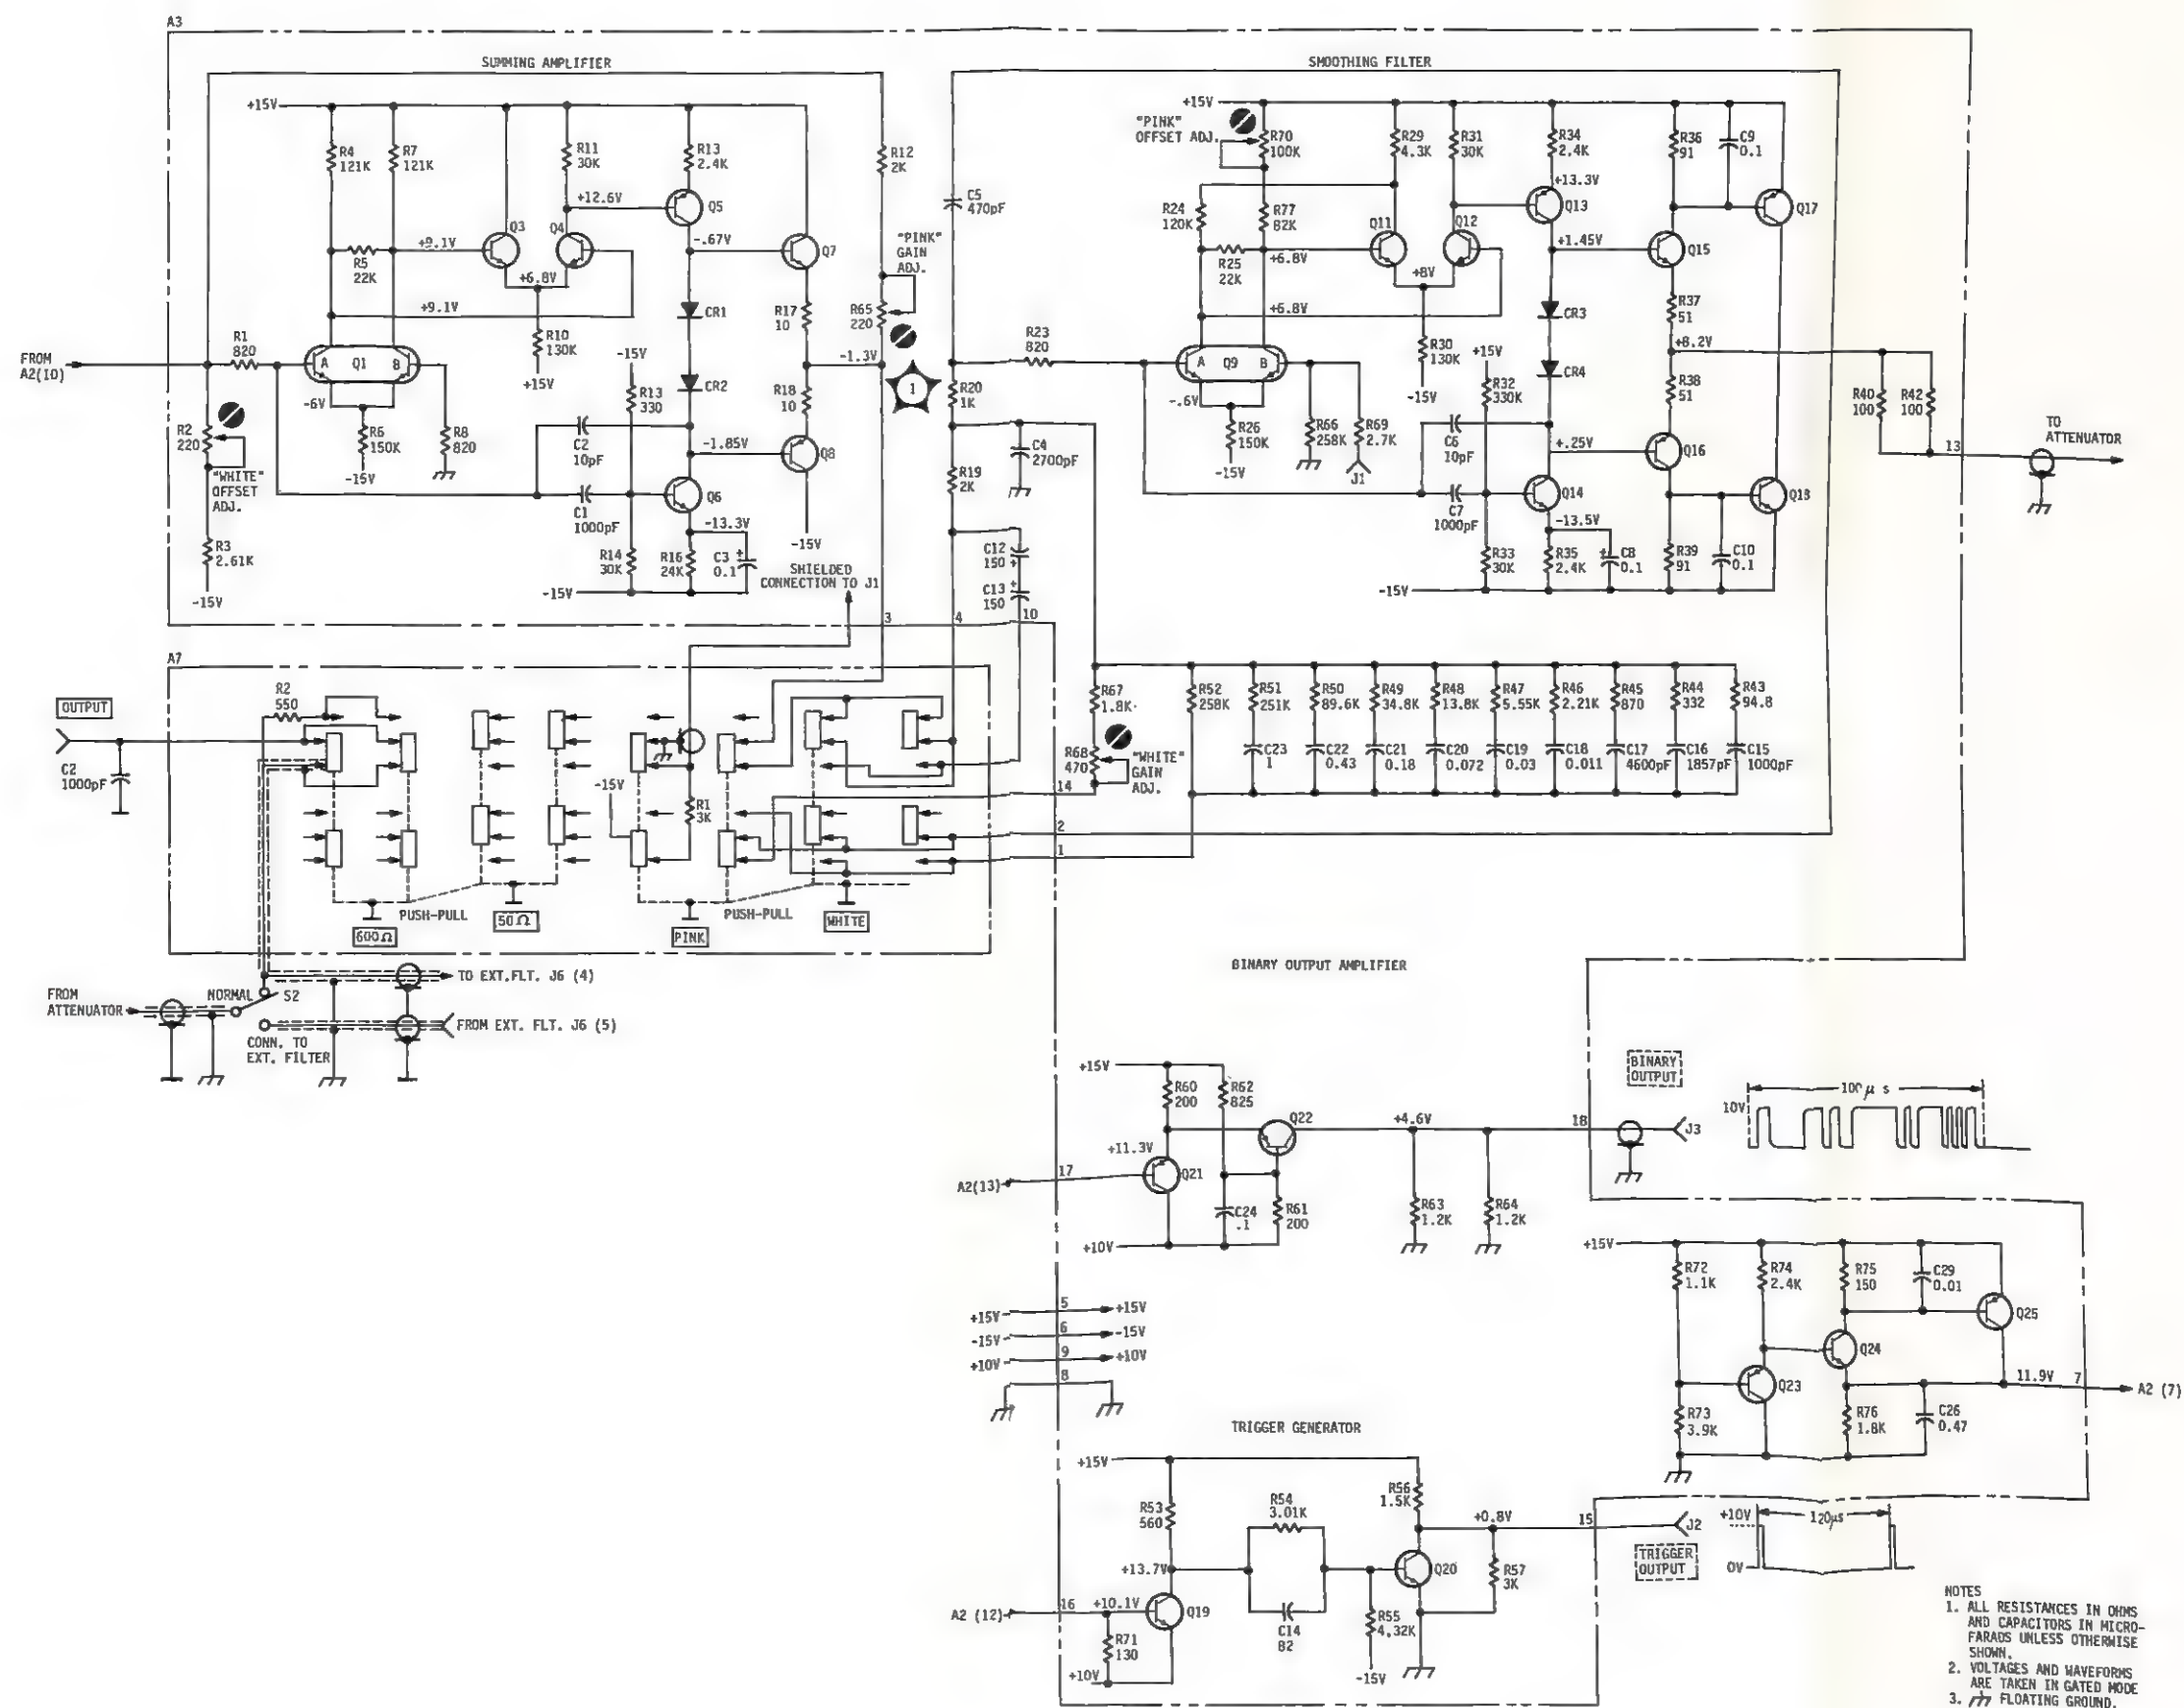


Figure 7-7 Assemblies 3 and 7 Circuit Diagram

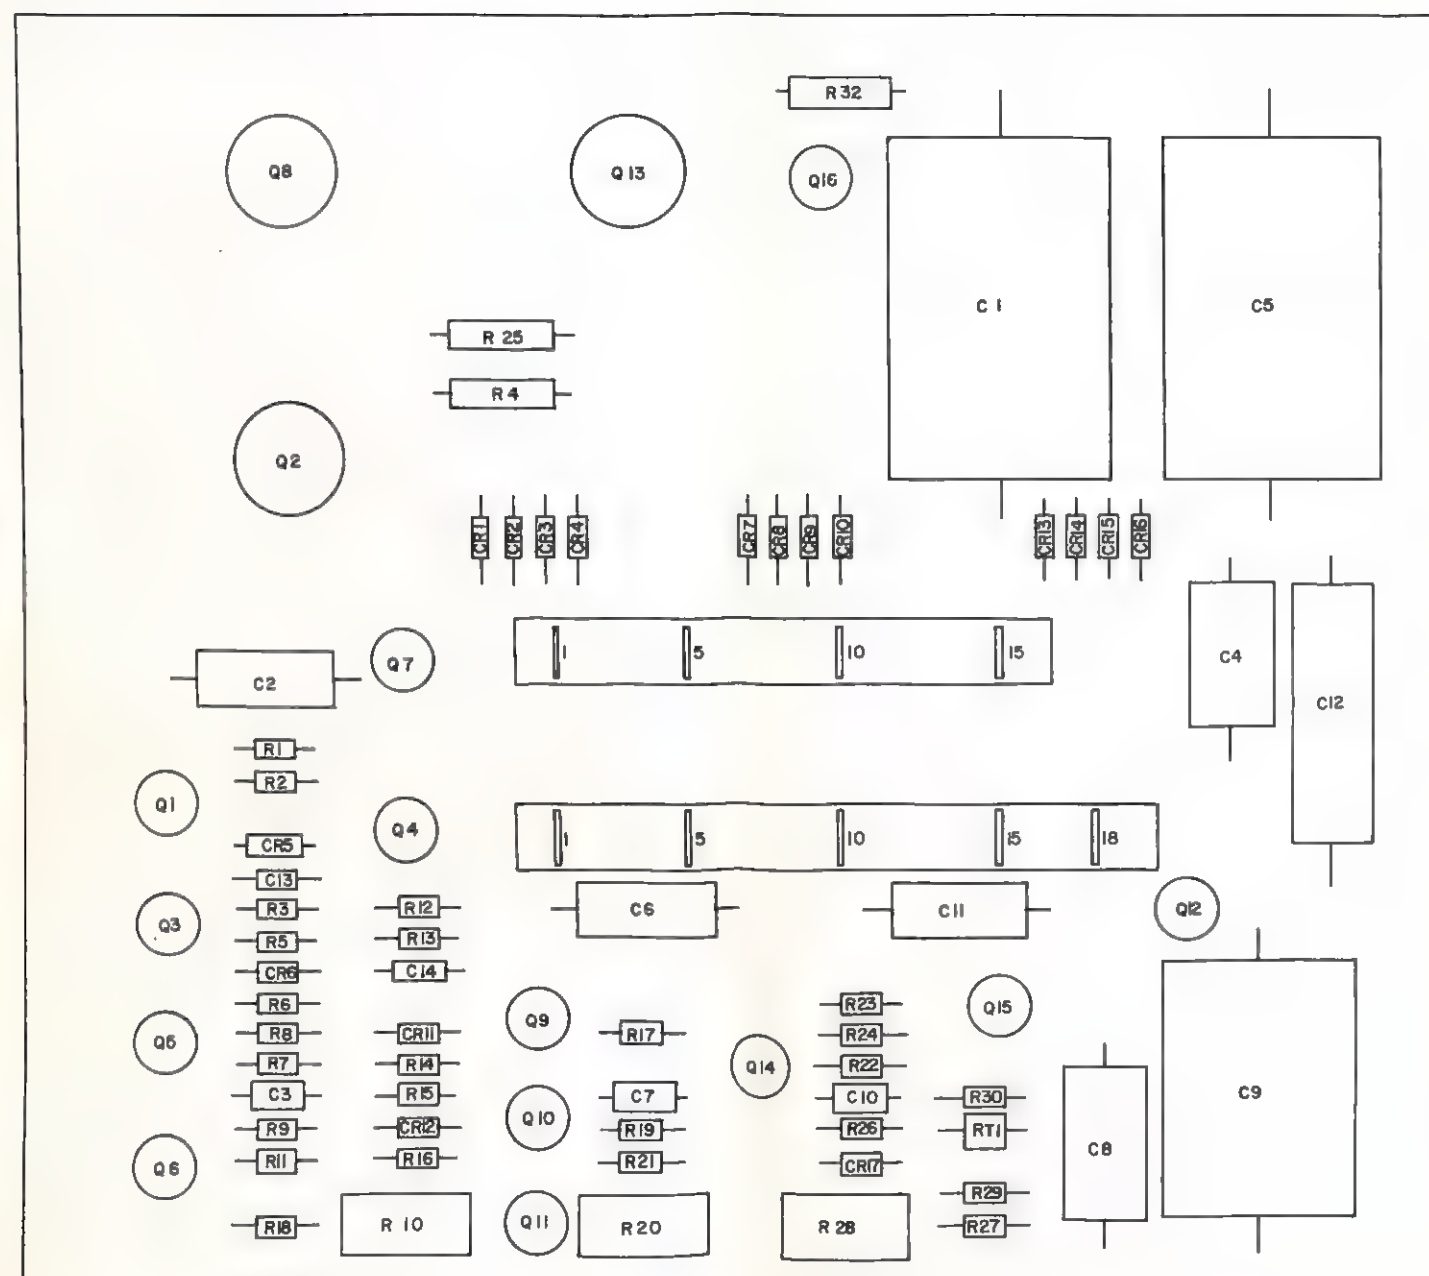


Figure 7-8 Assembly 1 Component Layout

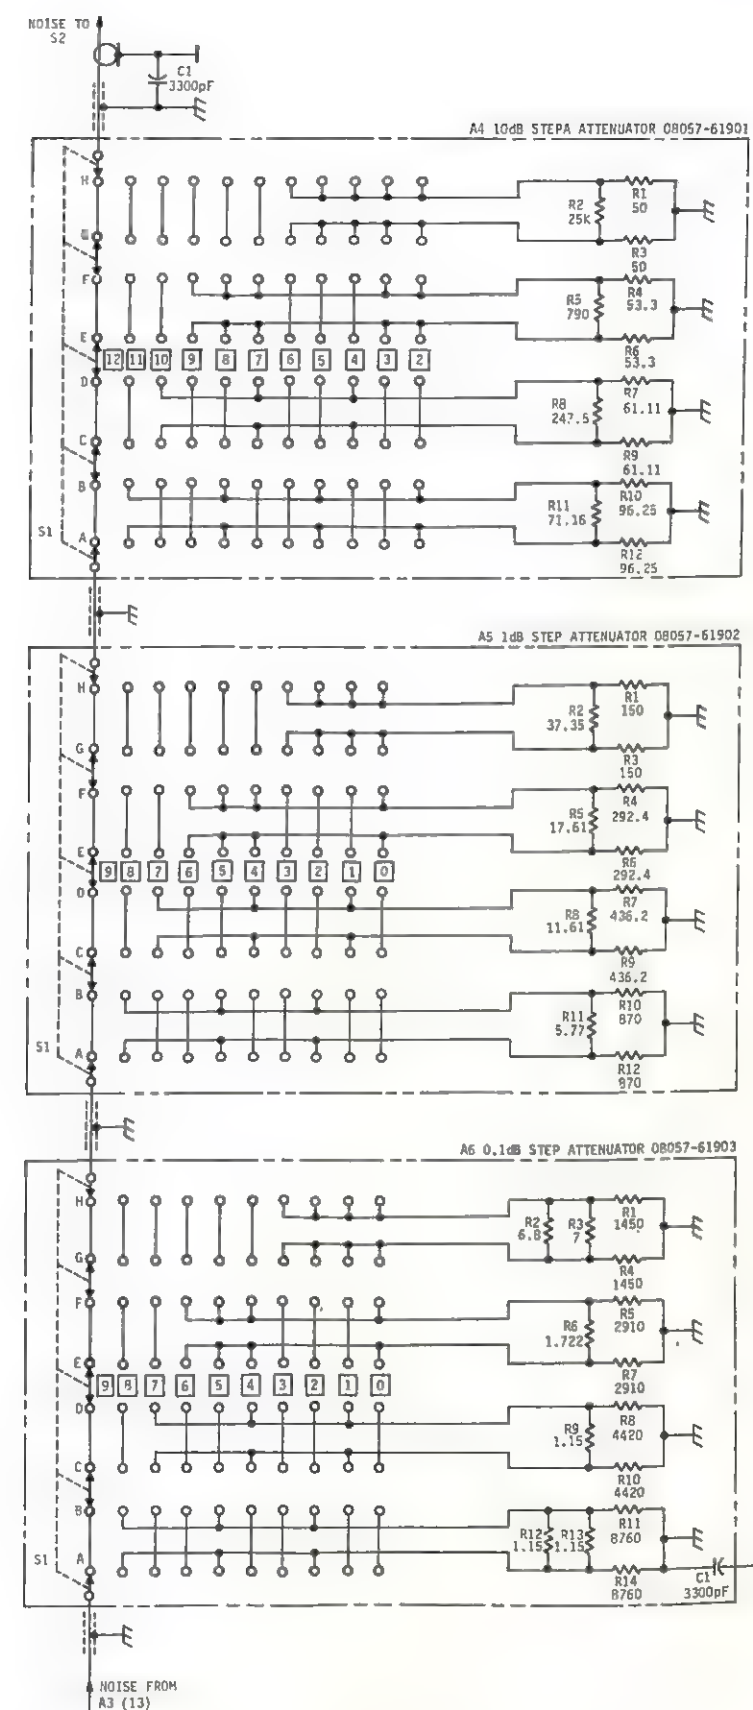


Figure 7-9 Assemblies 4, 5 and 6 Circuit Diagram


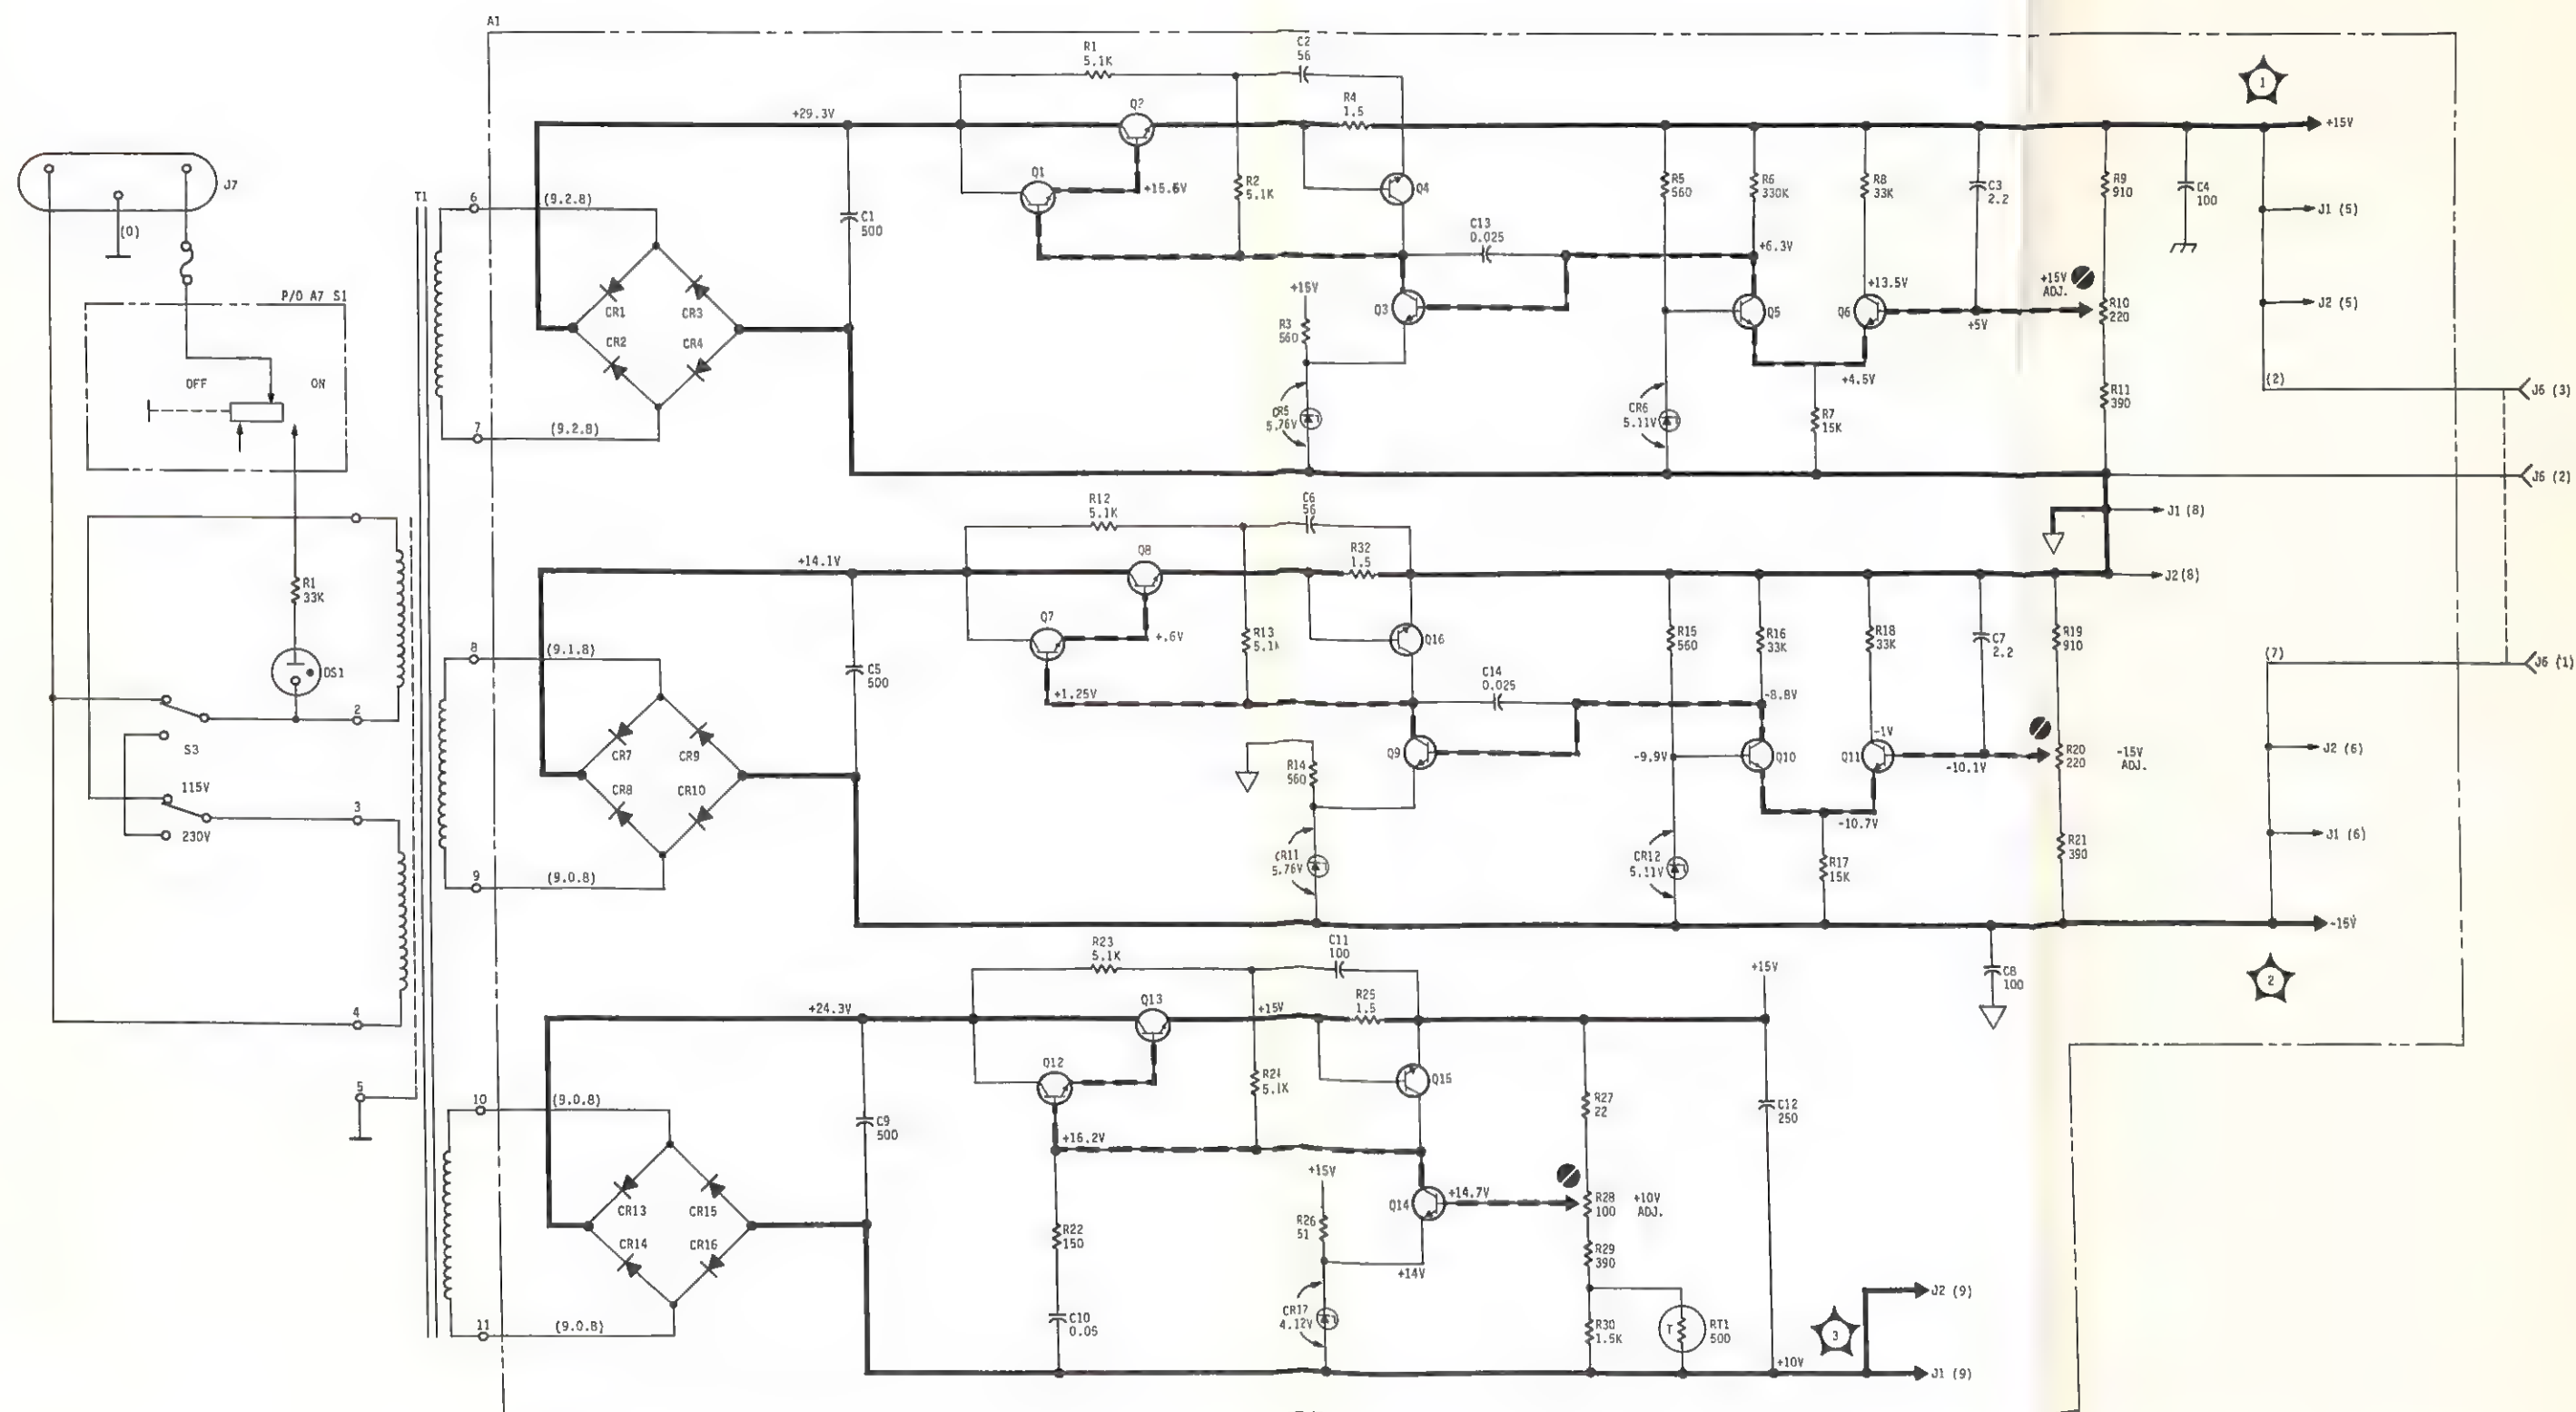


Figure 7-10 Assemblies 1 Circuit Diagram

A1-1 OPTION 001

A1-2 The 8057A Option 001 is the standard model with the attenuator removed. The output level available

at the external filter connector is fixed at 99.9dB. The output level at the output connector is fixed at 129.9dB. A circuit diagram of the parts unique to the Option 001 is shown in figure A1-1.

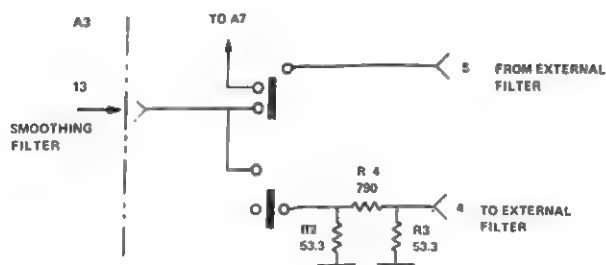

R2, 3	0698-6232	R:fxd, met flm 53.3Ω 1/8W
R4	0698-6230	R:fxd, met flm 790Ω 1/8W
	0360-0114	Terminal Strip
	08057-04102	Cover - Panel

Figure A1-1 Option 001 Circuit Diagram and Replaceable Parts

A1-3 OPTION A85

A1-4 The 8057A is available in light grey panels with olive case, instead of the standard livery, under this option number.

A1-5 OPTION X95

A1-6 The 8057A is available in light grey panels with blue case, instead of the standard livery, under this option number.



**A2-1 MODELS PRIOR TO SERIAL NUMBER
G910-00240****A2-2** These models were fitted with:

J7 Power connector 1251-2357
W1 Power cord 8120-1349

**A2-3 MODELS PRIOR TO SERIAL NUMBER
G910-00180****A2-4** These models were fitted with:

A2R113 R-F $3k\Omega$ 5% 0698-4265
(The present value of A2R113 ensures proper
operation of the external gate facility).

**A2-5 MODELS PRIOR TO SERIAL NUMBER
G910-00140****A2-6** These models were fitted with:

A2C2 C-F $2.2\mu F$ 0180-0197
(The present value of A2C2 ensures proper
operation of the auto-start circuit).

**A2-7 MODELS PRIOR TO SERIAL NUMBER
0963G 00390****A2-8** These models were supplied with light grey
panels and olive grey case.

SALES & SERVICE OFFICES

UNITED STATES

ALABAMA

P.O. Box 4207
2003 Byrd Spring Road S.W.
Huntsville 35802
Tel: (205) 881-4591
TWX: 810-726-2204

ARIZONA

2336 E. Magnolia St.
Phoenix 85034
Tel: (602) 252-5051
TWX: 910-951-1330

5737 East Broadway
Tucson 85716
Tel: (602) 298-2313
TWX: 910-952-1162

CALIFORNIA

1430 East Orangethorpe Ave.
Fullerton 92631
Tel: (714) 870-1000

3939 Lankershim Boulevard
North Hollywood 91604
Tel: (213) 877-1282
TWX: 910-499-2170

1101 Embarcadero Road
Palo Alto 94303
Tel: (415) 327-6500
TWX: 910-373-1280

2220 Watt Ave.
Sacramento 95825
Tel: (916) 482-1453
TWX: 910-367-2092

9606 Aero Drive
San Diego 92123
Tel: (714) 279-3200
TWX: 910-335-2000

COLORADO

7965 East Prentice
Englewood 80110
Tel: (303) 771-3455
TWX: 910-935-0705

CONNECTICUT

508 Tolland Street
East Hartford 06108
Tel: (203) 289-9394
TWX: 710-425-3416

111 East Avenue
Norwalk 06851
Tel: (203) 853-1251
TWX: 710-468-3750

FLORIDA

P.O. Box 24210
2806 W. Oakland Park Blvd.
Ft. Lauderdale 33307
Tel: (305) 731-2020
TWX: 910-955-4099

P.O. Box 20007
Herndon Station 32814
621 Commonwealth Avenue
Orlando
Tel: (305) 841-3970
TWX: 810-850-0113

Effective April 1, 1972
P.O. Box 13910
6177 Lake Ellenor Dr.
Orlando, 32809
Tel: (305) 859-2900
TWX: 810-850-0113

GEORGIA

P.O. Box 28234
450 Interstate North
Atlanta 30328
Tel: (404) 436-5181
TWX: 810-766-4890

ILLINOIS

5500 Howard Street
Skokie 60076
Tel: (312) 677-0400
TWX: 910-223-3613

INDIANA

3839 Meadows Drive
Indianapolis 46205
Tel: (317) 546-4891
TWX: 810-341-3263

LOUISIANA

P.O. Box 856
1942 Williams Boulevard
Kenner 70062
Tel: (504) 721-6201
TWX: 810-955-5524

MARYLAND

6707 Whitestone Road
Baltimore 21207
Tel: (301) 944-5400
TWX: 710-862-9157

P.O. Box 1648
2 Choke Cherry Road
Rockville 20850
Tel: (301) 948-6370
TWX: 710-828-9684

MASSACHUSETTS

32 Hartwell Ave.
Lexington 02173
Tel: (617) 861-8960
TWX: 710-326-6904

MICHIGAN

21840 West Nine Mile Road
Southfield 48075
Tel: (313) 353-9100
TWX: 810-224-4882

MINNESOTA

2459 University Avenue
St. Paul 55114
Tel: (612) 645-9461
TWX: 910-563-3734

MISSOURI

11131 Colorado Ave.
Kansas City 64137
Tel: (816) 763-8000
TWX: 910-771-2087

2812 South Brentwood Blvd.
St. Louis 63144
Tel: (314) 962-5000
TWX: 910-760-1670

NEW JERSEY

W. 120 Century Road
Paramus 07652
Tel: (201) 265-5000
TWX: 710-990-4951

1060 N. Kings Highway
Cherry Hill 08034
Tel: (609) 667-4000
TWX: 710-892-4945

NEW MEXICO

P.O. Box 8366
Station C
6501 Lomas Boulevard N.E.
Albuquerque 87108
Tel: (505) 265-3713
TWX: 910-989-1665

156 Wyatt Drive
Las Cruces 88001
Tel: (505) 526-2485
TWX: 910-983-0550

NEW YORK

1702 Central Avenue
Albany 12205
Tel: (518) 869-8462
TWX: 710-441-8270

1219 Campville Road
Endicott 13760
Tel: (607) 754-0050
TWX: 510-252-0890

82 Washington Street
Poughkeepsie 12601
Tel: (914) 454-7330
TWX: 510-248-0012

39 Saginaw Drive
Rochester 14623
Tel: (716) 473-9500
TWX: 510-253-5981

5858 East Molloy Road
Syracuse 13211
Tel: (315) 454-2486
TWX: 710-541-0482

1 Crossways Park West
Woodbury 11797
Tel: (516) 921-0300
TWX: 510-223-0811

NORTH CAROLINA

P.O. Box 5188
1923 North Main Street
High Point 27262
Tel: (919) 885-8101
TWX: 510-926-1516

OHIO

25575 Center Ridge Road
Cleveland 44145
Tel: (216) 835-0300
TWX: 810-427-9129

3460 South Dixie Drive
Dayton 45439
Tel: (513) 298-0351
TWX: 810-459-1925

1120 Morse Road
Columbus 43229
Tel: (614) 846-1300

OKLAHOMA

2919 United Founders Boulevard
Oklahoma City 73112
Tel: (405) 848-2801
TWX: 910-830-6862

OREGON

Westhills Mall, Suite 158
4475 S.W. Scholls Ferry Road
Portland 97225
Tel: (503) 292-9171
TWX: 910-464-6103

PENNSYLVANIA

2500 Moss Side Boulevard
Monroeville 15146
Tel: (412) 271-0724
TWX: 710-797-3650

1021 8th Avenue
King of Prussia Industrial Park
King of Prussia 19406
Tel: (215) 265-7000
TWX: 510-660-2870

RHODE ISLAND

873 Waterman Ave.
East Providence 02914
Tel: (401) 434-5535
TWX: 710-381-7573

*TENNESSEE

Memphis
Tel: (901) 274-7472

TEXAS

P.O. Box 1270
201 E. Arapaho Rd.
Richardson 75080
Tel: (214) 231-6101
TWX: 910-867-4723

P.O. Box 22813
6300 Westpark Drive
Suite 100
Houston 77027
Tel: (713) 781-6000
TWX: 910-881-2645

231 Billy Mitchell Road
San Antonio 78226
Tel: (512) 434-4171
TWX: 910-871-1170

UTAH

2890 South Main Street
Salt Lake City 84115
Tel: (801) 487-0715
TWX: 910-925-5681

VERMONT

P.O. Box 2287
Kennedy Drive
South Burlington 05401
Tel: (802) 458-4455
TWX: 510-299-0025

VIRGINIA

P.O. Box 6514
2111 Spencer Road
Richmond 23230
Tel: (703) 285-3431
TWX: 710-956-0157

WASHINGTON

433-108th N.E.
Bellevue 98004
Tel: (206) 454-3971
TWX: 910-443-2303

*WEST VIRGINIA

Charleston
Tel: (304) 768-1232

FOR U.S. AREAS NOT LISTED:

Contact the regional office nearest you: Atlanta, Georgia... North Hollywood, California... Paramus, New Jersey... Skokie, Illinois. Their complete addresses are listed above.

*Service Only

CANADA

ALBERTA

Hewlett-Packard (Canada) Ltd.
11745 Jasper Ave.
Edmonton
Tel: (403) 482-5561
TWX: 610-831-2431

BRITISH COLUMBIA

Hewlett-Packard (Canada) Ltd.
4519 Canada Way
North Burnaby 2
Tel: (604) 433-8213
TWX: 610-922-5059

MANITOBA

Hewlett-Packard (Canada) Ltd.
511 Bradford Ct.
Winnipeg
Tel: (204) 786-7581
TWX: 610-671-3531

NOVA SCOTIA

Hewlett-Packard (Canada) Ltd.
2745 Dutch Village Rd.
Suite 206
Halifax
Tel: (902) 455-0511
TWX: 610-271-4482

ONTARIO

Hewlett-Packard (Canada) Ltd.
880 Lady Ellen Place
Ottawa 3
Tel: (613) 255-6180, 255-6530
TWX: 610-562-1952

Hewlett-Packard (Canada) Ltd.
50 Galaxy Blvd.
Rexdale
Tel: (416) 677-9611
TWX: 610-492-4246

QUEBEC

Hewlett-Packard (Canada) Ltd.
275 Hymus Boulevard
Pointe Claire
Tel: (514) 697-4232
TWX: 610-422-3022
Telex: 01-20607

FOR CANADIAN AREAS NOT LISTED:

Contact Hewlett-Packard (Canada) Ltd. in Pointe Claire, at the complete address listed above.

CENTRAL AND SOUTH AMERICA

ARGENTINA

Hewlett-Packard Argentina
S.A.Ce.I
Lavalle 1171 - 3°
Buenos Aires
Tel: 35-0436, 35-0627, 35-0431
Telex: 012-1009
Cable: HEWPACKARG

BRAZIL

Hewlett-Packard Do Brasil
Lda. Ltda.
Rua Frei Caneca 1119
Sao Paulo - 3, SP
Tel: 288-7111, 287-5858
Cable: HEWPACK Sao Paulo

Hewlett-Packard Do Brasil
Praca Dom Feliciano 78
Salas 806/808
Porto Alegre
Rio Grande do Sul (RS)-Brasil
Tel: 25-8470
Cable: HEWPACK Porto Alegre

Hewlett-Packard Do Brasil
Lda. Ltda.
Rua da Matriz 29
Botafogo ZC-02
Rio de Janeiro, GB
Tel: 246-4417
Cable: HEWPACK Rio de Janeiro

CHILE

Héctor Calcagni y Cia, Ltda.
Bustos, 1932-3er Piso
Casilla 13942
Santiago
Tel: 423 96
Cable: CALCAGNI Santiago

COLOMBIA

Instrumentacion
Henrik A. Langebaek & Kier
Ltda.
Carrera 7 No. 48-59
Apartado Aereo 6287
Bogota, 1 D.E.
Tel: 45-78-06, 45-55-46
Cable: AARIS Bogota
Telex: 44400 INSTCO

COSTA RICA

Lic. Alfredo Gallegos Gurdán
Apartado 10159
San José
Tel: 21-86-13
Cable: GALGUR San José

ECUADOR

Laboratorios de Radio-Ingeniería
Calle Guayaquil 1246
Post Office Box 3199
Quito
Tel: 212-496; 219-185
Cable: HORVATH Quito

EL SALVADOR

Electronic Associates
Apartado Postal 1682
Centro Comercial Gigante
San Salvador, El Salvador
Paseo Escalon 4649-4th Piso
Tel: 23-44-60, 23-32-37
Cable: ELECAS

MEXICO

Hewlett-Packard Mexicana, S.A.
de C.V.
622 Adolfo Prieto
Col. del Valle
Mexico 12, D.F.
Tel: 543-4232; 523-1874
Telex: 0017-74507

NICARAGUA

Roberto Terán G.
Apartado Postal 689
Edificio Terán
Managua
Tel: 3451, 3452
Cable: ROTERAN Managua

PANAMA

Electrónica Balboa, S.A.
P.O. Box 4929
Ave. Manuel Espinosa No. 13-50
Bldg. Alina
Panama City
Tel: 230833
Telex: 3481003, Curundu,
Canal Zone
Cable: ELECTRON Panama City

PARAGUAY

Z.T. Melamed S.R.L.
Division: Aparatos y Equipos
Medicos
Salon de Exposición y Escritorio:
Chile 482
Edificio Victoria—Planta Baja
Asunción, Paraguay
Tel: 4-5069, 4-6272
Cable: RAMEL

PERU

Compañía Electro Medica S.A.
Ave. Enrique Canaval 312
San Isidro
Casilla 1030
Lima
Tel: 22-3900
Cable: ELMED Lima

PUERTO RICO

San Juan Electronics, Inc.
P.O. Box 5167
Ponce de Leon 154
Pda. 3-PTA de Tierra
San Juan 00906
Tel: (809) 725-3342, 722-3342
Cable: SATRONICS San Juan
Telex: SATRON 3450 332

SURINAME

Surfel-Radio Holland N.V.
P.O. Box 155
Paramaribo
Tel: 72118
Cable: Treurniet Paramaribo

URUGUAY

Pablo Ferrando S.A.
Comercial e Industrial
Avenida Italia 2877
Casilla de Correo 370
Montevideo
Tel: 40-3102
Cable: RADIUM Montevideo

VENEZUELA

Hewlett-Packard De Venezuela
C.A.
Apartado 50933
Caracas
Tel: 71.88.05, 71.88.69, 71.99.30
Cable: HEWPACK Caracas
Telex: 39521146

FOR AREAS NOT LISTED,

CONTACT:
Hewlett-Packard
INTERCONTINENTAL
3200 Hillview Ave.
Palo Alto, California 94304
Tel: (415) 493-1501
TWX: 910-373-1267
Cable: HEWPACK Palo Alto
Telex: 034-8461

EUROPE

AUSTRIA
Hewlett-Packard Ges.m.b.H
Innstrasse 23/2
Postfach 45
A-1204 Vienna
Tel: (0222) 33 66 06-09
Cable: HEWPAK Vienna
Telex: 75923 hewpak a

BELGIUM
Hewlett-Packard Benelux
S.A./N.V.
Avenue du Col-Vert, 1
B-1170 Brussels
Tel: (02) 72 22 40
Cable: PALOBEN Brussels
Telex: 23 494

DENMARK
Hewlett-Packard A/S
Datavej 38
DK-3460 Birkerød
Tel: (01) 81 66 40
Cable: HEWPAK AS
Telex: 16640 hp as

Hewlett-Packard A/S
Torvet 9
DK-8600 Silkeborg
Tel: (08) 82-71-66
Telex: 16640 hp as
Cable: HEWPAKAS

FINLAND
Hewlett-Packard Oy
Bulevardi 26
P.O. Box 12185
SF-00120 Helsinki 12
Tel: 13-730
Cable: HEWPAKOV-Helsinki
Telex: 12-1563

FRANCE
Hewlett-Packard France
Quartier de Courtaboeuf
Boite Postale No. 6
F-91 Orsay
Tel: (1) 907 78 25
Cable: HEWPAK Orsay
Telex: 60048

Hewlett-Packard France
4 Quai des Etoiles
F-69 Lyon 5ème
Tel: (78) 42 63 45
Cable: HEWPAK Lyon
Telex: 31617

**GERMAN FEDERAL
REPUBLIC**
Hewlett-Packard Vertriebs-GmbH
Berliner Strasse 117
Postfach 560/40
D-6 Nieder-Eschbach/Ffm 56
Tel: (0611) 50-04-1
Cable: HEWPAKSA Frankfurt
Telex: 41 32 49 FRA

Hewlett-Packard Vertriebs-GmbH
Herrenbergerstrasse 110
D-7030 Böblingen, Württemberg
Tel: (07031) 66 72 86
Cable: HEPAK Böblingen
Telex: 72 65 739

Hewlett-Packard Vertriebs-GmbH
Vogelsanger Weg 38
D-4 Büsselfeld
Tel: (0211) 63 80 31/35
Telex: 85/86 533

Hewlett-Packard Vertriebs-GmbH
Wendenstr. 23
D-2 Hamburg 1
Tel: (0411) 24 05 51/52
Cable: HEWPAKSA Hamburg
Telex: 21 53 32

Hewlett-Packard Vertriebs-GmbH
Unterhachinger Strasse 28
ISAR Center
D-8012 Ottobrunn
Tel: (0811) 60 13 061-7
Telex: 05-24985
Cable: HEWPAKSA München
(West Berlin)
Hewlett-Packard Vertriebs-GmbH
Wilmersdorfer Strasse 113/114
D-1000 Berlin W. 12
Tel: (0311) 3137046
Telex: 18 34 05

GREECE
Kostas Karayannis
18, Ermou Street
Athens 126
Tel: 230301,3,5
Cable: RAKAR Athens
Telex: 21 59 62 RKAR GR

IRELAND
Hewlett-Packard Ltd.
224 Bath Road
Slough, SL1 4 DS, Bucks
Tel: Slough 753-33341
Cable: HEWPIE Slough
Telex: 84413

ITALY
Hewlett-Packard Italiana S.p.A.
Via Amerigo Vespucci 2
I-20124 Milan
Tel: (2) 6251 (10 lines)
Cable: HEWPAKIT Milan
Telex: 32046
Hewlett-Packard Italiana S.p.A.
Via Marocco, 7
I-00144 Rome - Eur
Tel: (6) 5912544/5, 5915947
Cable: HEWPAKIT Rome
Telex: 61514

LUXEMBURG
Hewlett-Packard Benelux
S.A./N.V.
Avenue du Col-Vert, 1
B-1170 Brussels
Tel: (03/02) 72 22 40
Cable: PALOBEN Brussels
Telex: 23 494

NETHERLANDS
Hewlett-Packard Benelux, N.V.
Weerdestein 117
P.O. Box 7825
Amsterdam, Z 11
Tel: 020-42 77 77
Cable: PALOBEN Amsterdam
Telex: 13 216

NORWAY
Hewlett-Packard Norge A/S
Box 149
Nesveien 13
N-1344 Haslum
Tel: (02)-53 83 60
Telex: 16621

PORTUGAL
Teletra-Empresa Tecnica de
Equipamentos
Electricos S.a.r.l.
Rua Rodrigo da Fonseca 103
P.O. Box 2531
Lisbon 1
Tel: 68 60 72
Cable: TELETRA Lisbon
Telex: 1598

SPAIN
Hewlett-Packard Española, S.A.
Jerez No 8
Madrid 16
Tel: 458 26 00

SWEDEN
Hewlett-Packard Sverige AB
Enighetsvägen 1-3
Fack
S-161 20 Bromma 20
Tel: (08) 98 12 50
Cable: MEASUREMENTS
Stockholm
Telex: 10721

Hewlett-Packard Sverige AB
Hagakersgatan 9C
S-431 41 Mölndal
Tel: (031) 27 68 00/01
Telex: 21 312 hpmindls

SWITZERLAND
Hewlett Packard (Schweiz) AG
Zürcherstrasse 20
CH-8952 Schlieren Zurich
Tel: (01) 98 18 21/24
Cable: HPAG CH
Telex: 53933

Hewlett-Packard (Schweiz) AG
Rue du Bois-du-Lan 7
P.O. Box 85
1217 Meyrin 2 Geneva
Tel: (022) 41 54 00
Cable: HEWPAKSA Geneva
Telex: 27333 HPAS CH

TURKEY
Telekom Engineering Bureau
P.O. Box 376
Karaköy
Istanbul
Tel: 49 40 40
Cable: TELEMAN Istanbul

UNITED KINGDOM
Hewlett-Packard Ltd.
224 Bath Road
Slough, SL1 4 DS, Bucks
Tel: Slough (0753) 33341
Cable: HEWPIE Slough
Telex: 84413
Hewlett-Packard Ltd.
"The Graftons"
Stamford New Road
Altrincham, Cheshire
Tel: (061) 928-8626
Telex: 688068

YUGOSLAVIA
Belram S.A.
83 avenue des Mimosas
Brussels 1150, Belgium
Tel: 34 33 32, 34 26 19
Cable: BELRAMEL Brussels
Telex: 21790

**SOCIALIST COUNTRIES
PLEASE CONTACT:**
Hewlett-Packard Ges.m.b.H
Innstrasse 23/2
Postfach 45
A-1204 Vienna, Austria
Tel: (0222) 33 66 06-09
Cable: HEWPAK Vienna
Telex: 75923 hewpak a

**ALL OTHER EUROPEAN
COUNTRIES CONTACT:**
Hewlett-Packard S.A.
Rue du Bois-du-Lan 7
1217 Meyrin 2 Geneva
Switzerland
Tel: (022) 41 54 00
Cable: HEWPAKSA Geneva
Telex: 2.24.86

AFRICA, ASIA, AUSTRALIA

ANGOLA
Teletra Empresa Técnica
de Equipamentos Eléctricos
SAR
Rua de Barbosa Rodrigues
42-1º
Box 6487
Luanda
Cable: TELETRA Luanda

AUSTRALIA
Hewlett-Packard Australia
Pty. Ltd.
22-26 Weir Street
Glen Iris, 3146
Victoria
Tel: 20.1371 (6 lines)
Cable: HEWPAK Melbourne
Telex: 31024

Hewlett-Packard Australia
Pty. Ltd.
61 Alexander Street
Crows Nest 2065
New South Wales
Tel: 43.7866
Cable: HEWPAK Sydney
Telex: 21561

Hewlett-Packard Australia
Pty. Ltd.
97 Churchill Road
Prospect 5082
South Australia
Tel: 65.2366
Cable: HEWPAK Adelaide

Hewlett Packard Australia
Pty. Ltd.
2nd Floor, Suite 13
Casablanca Buildings
196 Adelaide Terrace
Perth, W.A. 6000
Tel: 21-3330
Cable: HEWPAK Perth

Hewlett-Packard Australia
Pty. Ltd.
10 Woolley Street
P.O. Box 191
Dickson A.C.T. 2602
Tel: 49-8194
Cable: HEWPAK Canberra ACT

Hewlett-Packard Australia
Pty. Ltd.
6 Harward Street
P.O. Box 135
Kenmore 4069 Queensland
Tel: 78 6069

CEYLON
United Electricals Ltd.
P.O. Box 681
Yahala Building
Staples Street
Colombo 2
Tel: 5496
Cable: HOTPOINT Colombo

CYPRUS
Kyronics
19 Gregorios & Xenopoulos Road
P.O. Box 1152
Nicosia
Tel: 6282-75628
Cable: HE-I-NAMI

ETHIOPIA
African Salespower & Agency
Private Ltd., Co.
P.O. Box 718
58/59 Cunningham St.
Addis Ababa
Tel: 12285
Cable: ASACO Addisababa

HONG KONG
Schmidt & Co. (Hong Kong) Ltd.
P.O. Box 297
1511, Prince's Building 15th Floor
10, Chater Road
Hong Kong
Tel: 240168, 232735
Cable: SCHMIDTCO Hong Kong

INDIA
Blue Star Ltd.
Kasturji Buildings
Jamschadi Tata Rd.
Bombay 20BR, India
Tel: 29 50 21
Telex: 2156
Cable: BLUEFROST

Blue Star Ltd.
Band Box House
Prabhadevi
Bombay 25DD, India
Tel: 45 73 01
Telex: 2156
Cable: BLUESTAR

Blue Star Ltd.
14/40 Civil Lines
Kanpur, India
Tel: 6 88 82
Cable: BLUESTAR

Blue Star, Ltd.
7 Hare Street
P.O. Box 506
Calcutta 1, India
Tel: 23-0131
Telex: 655
Cable: BLUESTAR

Blue Star Ltd.
Blue Star House,
34 Ring Road
Lajpat Nagar
New Delhi 24, India
Tel: 62 32 76
Telex: 463
Cable: BLUESTAR

Blue Star Ltd.
17-C Ulsoor Road
Bangalore-8

Blue Star, Ltd.
96 Park Lane
Secunderabad 3, India
Tel: 7 63 91
Cable: BLUEFROST
Blue Star, Ltd.
23/24 Second Line Beach
Madras 1, India
Tel: 2 39 55
Telex: 379
Cable: BLUESTAR
Blue Star, Ltd.
18 Kaiser Bungalow
Dindli Road
Jamschadpur, India
Tel: 38 04
Cable: BLUESTAR

INDONESIA
Bah Bolon Trading Coy. N.V.
Djalat Merdeka 29
Bandung
Tel: 4915; 51560
Cable: ILMI
Telex: 08-809

IRAN
Telecom, Ltd.
P.O. Box 1812
240 Kh. Saba Shomali
Teheran
Tel: 43850, 48111
Cable: BASCOM Teheran
Telex: 2664

ISRAEL
Electronics & Engineering
Div. of Motorola Israel Ltd.
17 Aminadav Street
Tel-Aviv
Tel: 36941 (3 lines)
Cable: BASTEL Tel-Aviv
Telex: Bastei Tv 033-569

JAPAN
Yokogawa-Hewlett-Packard Ltd.
Ohashi Building
1-59-1 Yoyogi
Shibuya-Ku, Tokyo
Tel: 03-370-2281/7
Telex: 232-2024YHP
Cable: YHPMARKET TOK 23-724

Yokogawa-Hewlett-Packard Ltd.
Nisei Ibaragi Bldg.
2-2-8 Kasuga
Ibaragi-Shi
Osaka -
Tel: (0726) 23-1641
Telex: 385-5332 YHPOSACA

Yokogawa-Hewlett-Packard Ltd.
Ito Building
No. 59, Kotori-cho
Nakamura-ku, Nagoya City
Tel: (052) 551-0215

Yokogawa-Hewlett-Packard Ltd.
Nitto Bldg.
2300 Shinohara-cho,
Kohoku-ku
Yokohama 222
Tel: (405) 432-1504/5

JORDAN
Constantin E. Macridis
Clemenceau Street
P.O. Box 7213
Beirut, Lebanon
Tel: 220846
Cable: ELECTRONUCLEAR Beirut

KENYA
Kenya Kinetics
P.O. Box 18311
Nairobi, Kenya
Tel: 57726
Cable: PROTON

KOREA
American Trading Co.,
Korea, Ltd.
Seoul P.O. Box 1103
7th & 8th floors, DaeKyung Bldg.
107 Sejong Ro
Chongro-Ku, Seoul
Tel: 75-5841 (4 lines)
Cable: AMTRACO Seoul

LEBANON
Constantin E. Macridis
Clemenceau Street
P.O. Box 7213
Beirut
Tel: 220846
Cable: ELECTRONUCLEAR Beirut

MALAYSIA
MECOMB Malaysia Ltd.
2 Larong 13/6A
Section 13
Petaling Jaya, Selangor
Cable: MECOMB Kuala Lumpur

MOZAMBIQUE
A. N. Goncalves, LDA.
4.1 Apt. 14 Av. D. Luis
P.O. Box 107
Lourenco Marques
Cable: NEGON

NEW ZEALAND
Hewlett-Packard (N.Z.) Ltd.
94-96 Dixon St.
P.O. Box 9443
Wellington, N.Z.
Tel: 56-559
Cable: HEWPAK Wellington

Hewlett Packard (N.Z.) Ltd.
Box 51092
Pukuranga
Tel: 569-651
Cable: HEWPAK Auckland

PAKISTAN (EAST)
Mushko & Company, Ltd.
1, Jinnah Avenue
Dacca 2
Tel: 280058
Cable: NEWDEAL Dacca

PAKISTAN (WEST)
Mushko & Company, Ltd.
Oosman Chambers
Abdullah Haroon Road
Karachi 3
Tel: 511027, 512927
Cable: COOPERATOR Karachi
Tel: 389160, 1, 2, 375121,
Corp. Bldg. 7th Floor
Taipei
Tel: 240
Telex: TP824 HEWPAK
Cable: HEWPAK Taipei

PHILIPPINES
Electromex Inc.
5th Floor, Architects
Center Bldg.
Ayala Ave., Makati, Rizal
C.C.P.O. Box 1028
Makati, Rizal
Tel: 86-18-87, 87-76-77
Cable: ELEMEX Manila

SINGAPORE
Mechanical and Combustion
Engineering Company Ltd.
9, Jalan Kilang
Red Hill Industrial Estate
Singapore, 3
Tel: 642361-3; 632611
Cable: MECOMB Singapore

Hewlett-Packard Far East
Area Office
P.O. Box 87
Alexandra Post Office
Singapore 3
Tel: 633022
Cable: HEWPAK SINGAPORE

SOUTH AFRICA
Hewlett Packard South Africa
(Pty.), Ltd.
P.O. Box 31716
Braamfontein Transvaal
Milnerton
30 De Beer Street
Johannesburg
Tel: 725-2080, 725-2030
Telex: 0226 JH
Cable: HEWPAK Johannesburg

Hewlett Packard South Africa
(Pty.), Ltd.
Breechle House
Bree Street
Cape Town
Tel: 3-6019, 3-6545
Cable: HEWPAK Cape Town
Telex: 5-0006

Hewlett Packard South Africa
(Pty.), Ltd.
641 Ridge Road, Durban
P.O. Box 99
Overport, Natal
Tel: 88-6102
Telex: 567954
Cable: HEWPAK

TAIWAN
Hewlett Packard Taiwan
39 Chung Shiao West Road
Sec. 1
Overseas Insurance
Corp. Bldg. 7th Floor
Taipei
Tel: 389160, 1, 2, 375121,
Ext. 240
Telex: TP824 HEWPAK
Cable: HEWPAK Taipei

THAILAND
The International
Engineering Co., Ltd.
P.O. Box 39
614 Sukhumvit Road
Bangkok
Tel: 910722 (7 lines)
Cable: GYSOM
TLX INTENCO BK-226 Bangkok

UGANDA
Uganda Tele-Electric Co., Ltd.
P.O. Box 4449
Kampala
Tel: 57279
Cable: COMCO Kampala

VIETNAM
Peninsular Trading Inc.
P.O. Box H-3
216 Hien-Vuong
Saigon
Tel: 20805, 93398
Cable: PENTRA, SAIGON 242

ZAMBIA
R. J. Tilbury (Zambia) Ltd.
P.O. Box 2792
Lusaka
Zambia, Central Africa
Tel: 73793
Cable: ARJAYTEE, Lusaka

**MEDITERRANEAN AND
MIDDLE EAST COUNTRIES
NOT SHOWN PLEASE
CONTACT:**
Hewlett-Packard
Co-ordination Office for
Mediterranean and Middle
East Operations
Via Marocco, 7
I-00144 Rome-Eur, Italy
Tel: (6) 59 40 29
Cable: HEWPAKIT Rome
Telex: 61514

**OTHER AREAS NOT
LISTED, CONTACT:**
Hewlett-Packard
INTERCONTINENTAL
3200 Hillview Ave.
Palo Alto, California 94304
Tel: (415) 326-7000
(Feb. 71 493-1501)
TWX: 910-373-1267
Cable: HEWPAK Palo Alto
Telex: 034-8461

